


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101124\
Data File : BN034551.D
Acq On : 11 Oct 2024 11:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Oct 11 00:21:08 2024

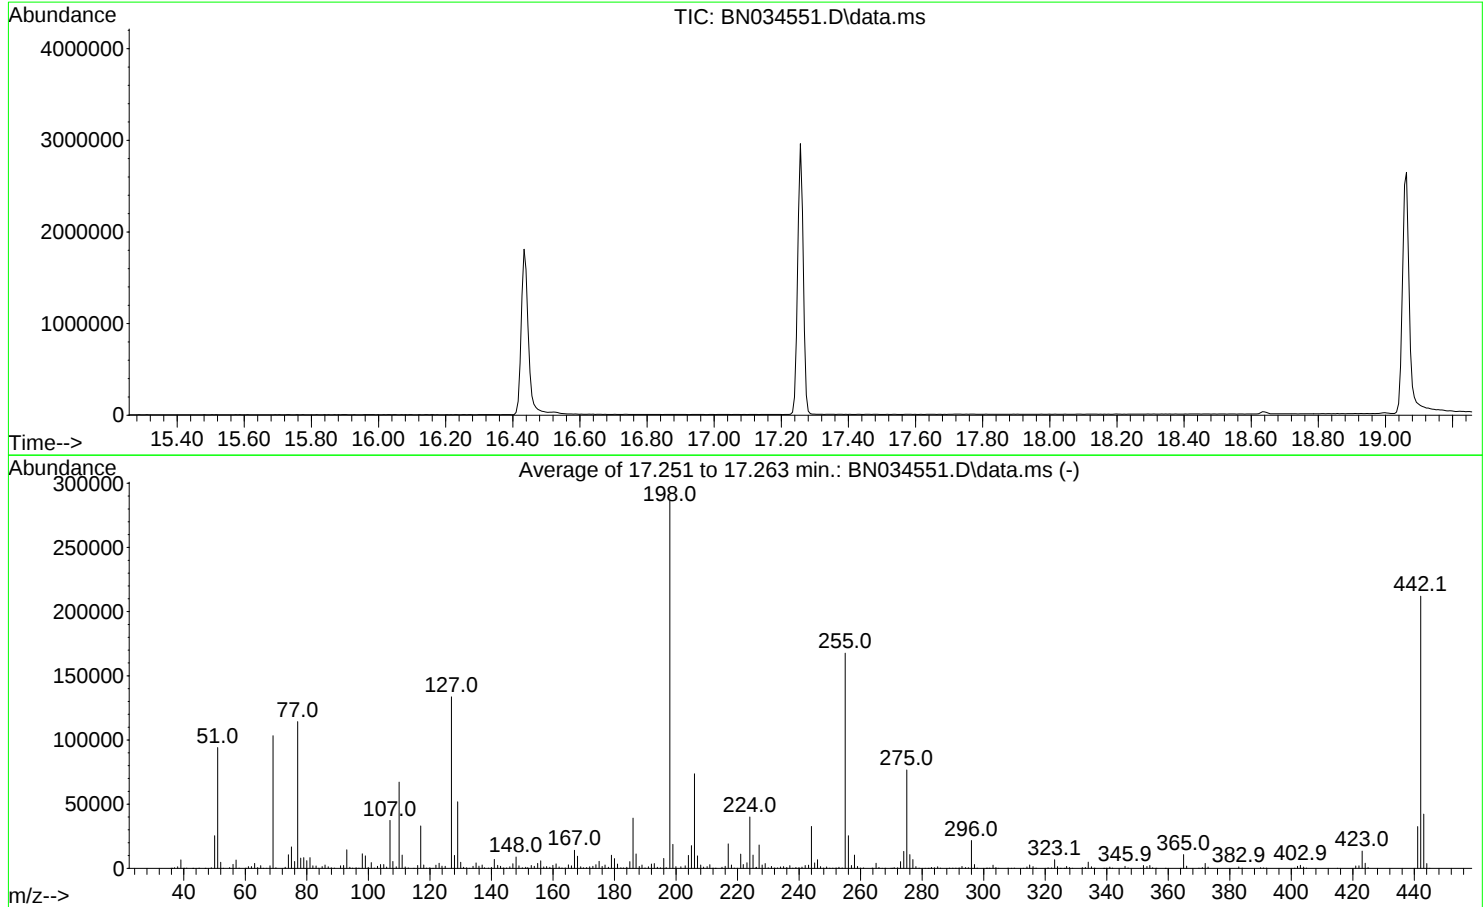

AutoFind: Scans 2442, 2443, 2444; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	94085	PASS
68	69	0.00	2	1.9	1958	PASS
69	198	0.00	100	36.1	103312	PASS
70	69	0.00	2	0.5	478	PASS
127	198	10	80	46.6	133595	PASS
197	198	0.00	2	0.2	633	PASS
198	198	100	100	100.0	286571	PASS
199	198	5	9	6.5	18742	PASS
275	198	10	60	26.7	76651	PASS
365	198	1	100	3.7	10682	PASS
441	198	0.01	100	11.4	32555	PASS
442	442	50	100	100.0	212011	PASS
443	442	15	24	20.0	42317	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/11/2024	BNA_N	<u>BN034551.D</u>
Compound Name	Response	Retention Time
DDT	911420	20.31
DDD	22548	19.869
DDE	1043	19.357
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23591	935011	2.52

Instrument :
BNA_N
ClientSampleId :
DFTPP

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:52:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

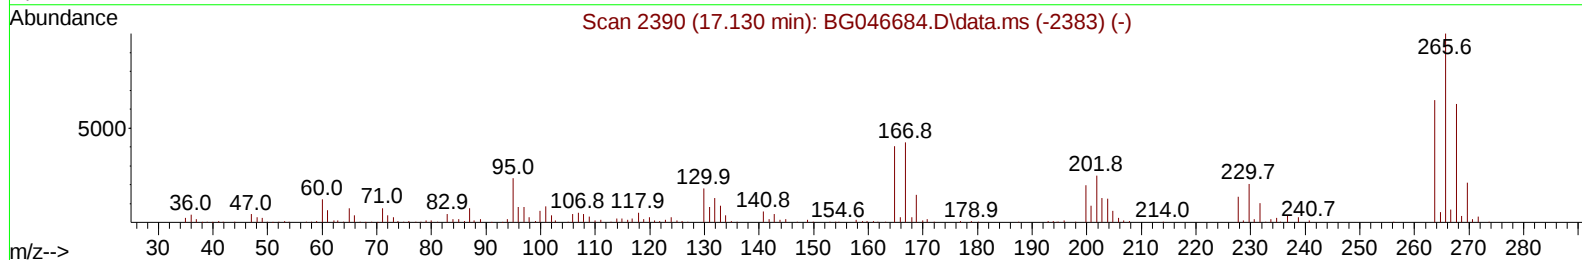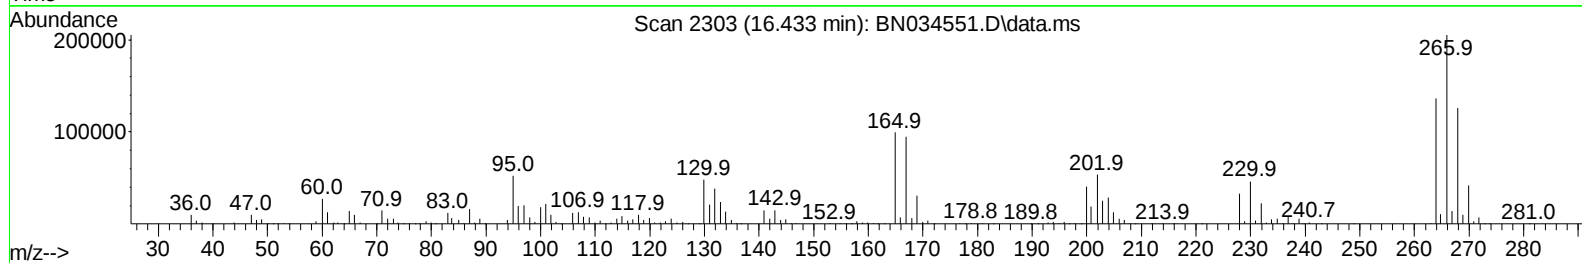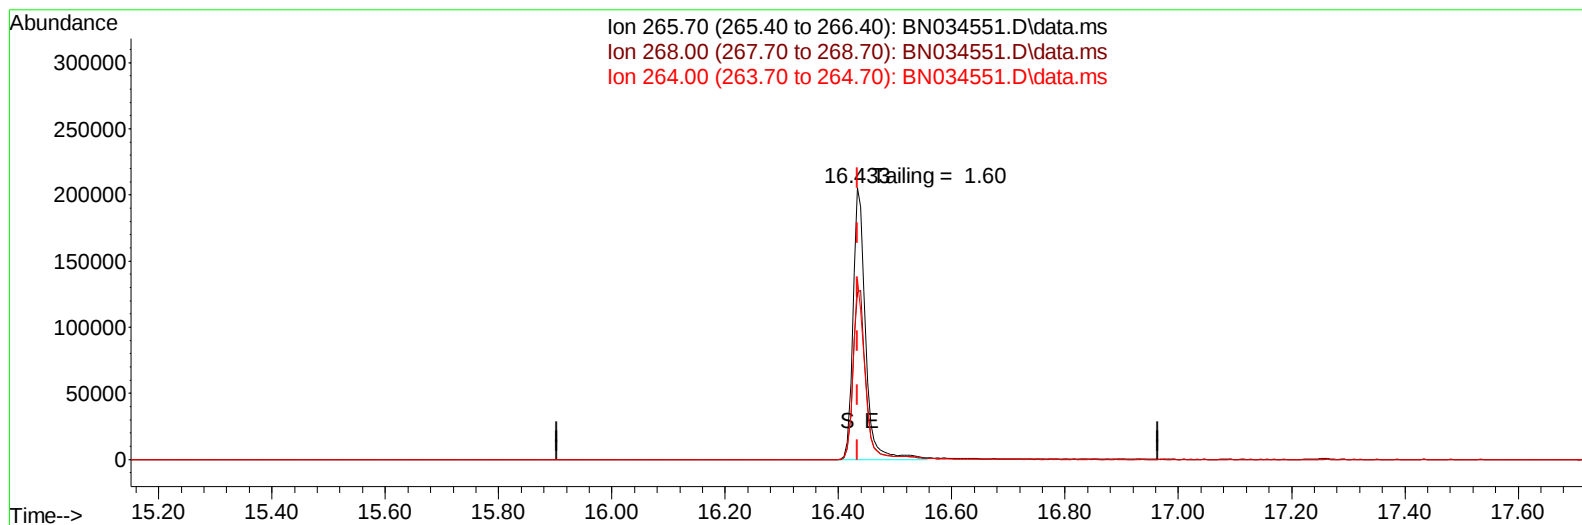

TIC: BN034551.D\data.ms

16.433min (0.000) 21872.07 ng




response **308792**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.49
264.00	61.60	66.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101124\
Data File : BN034551.D
Acq On : 11 Oct 2024 11:07
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 14 02:52:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 14 02:51:59 2024
Response via : Initial Calibration

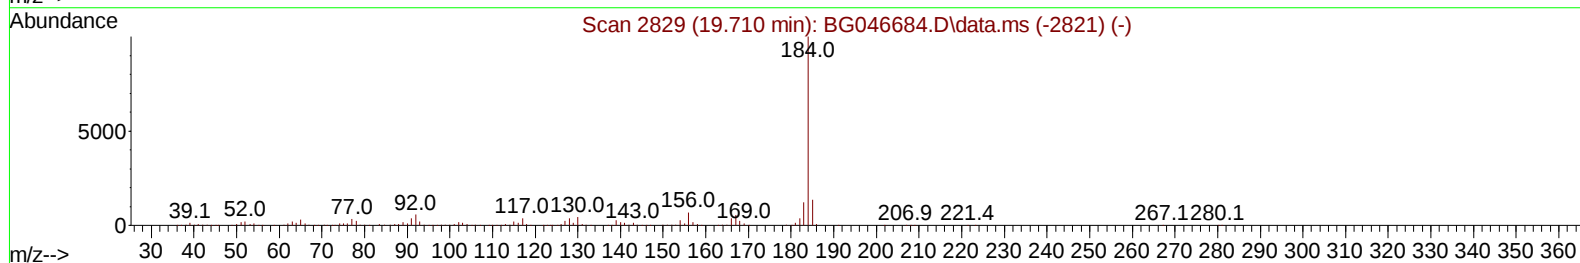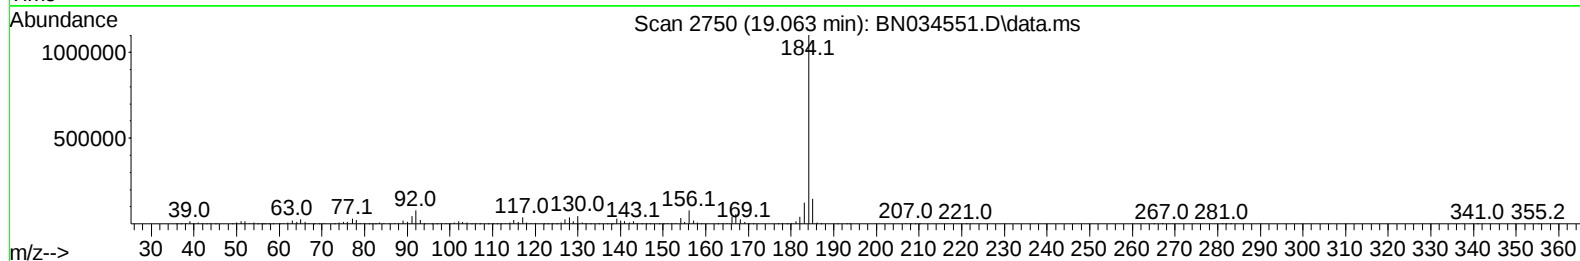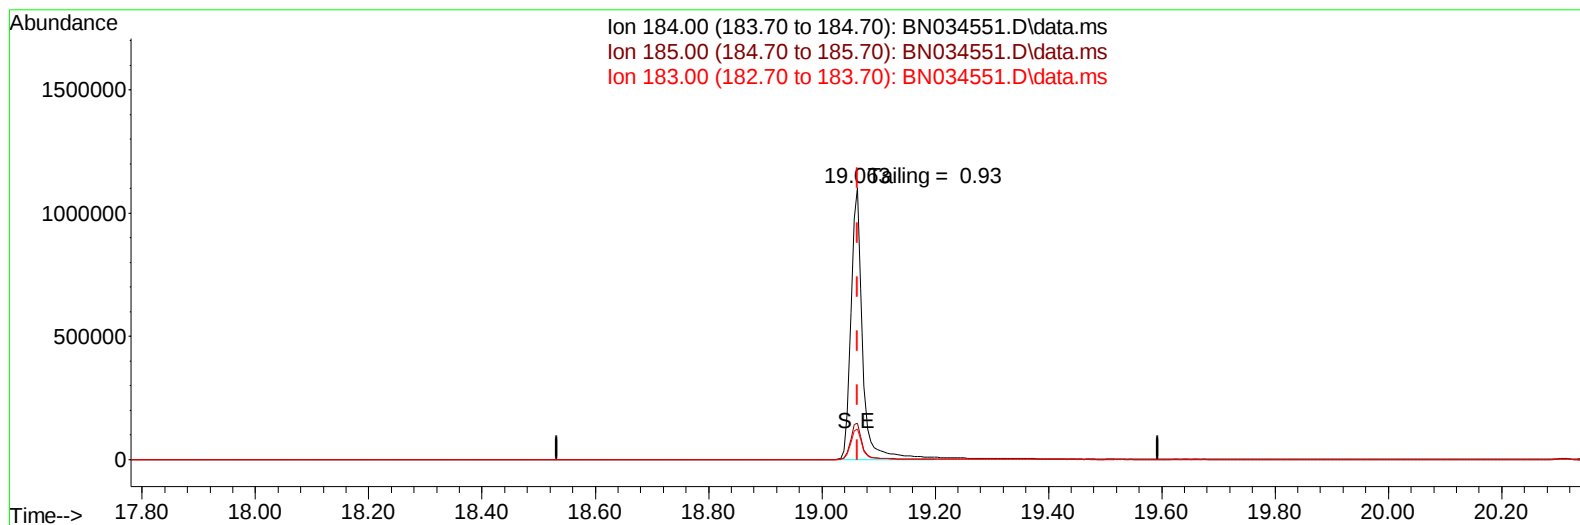

TIC: BN034551.D\data.ms

(77) Benzidine

19.063min (0.000) 0.00 ng

response 1587831

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.30
183.00	13.20	11.28
0.00	0.00	0.00