

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101220\
 Data File : BN012146.D
 Acq On : 12 Oct 2020 11:50
 Operator : CG/JU
 Sample : PB132270BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB132270BS

Manual Integrations
 APPROVED

mohammad
 10/13/2020 11:08:33 AM

Quant Time: Oct 12 12:19:11 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 12 11:15:56 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.635	152	1645	0.40	ng	0.00
7) Naphthalene-d8	10.402	136	6779	0.40	ng	# 0.00
13) Acenaphthene-d10	14.268	164	3746	0.40	ng	0.00
19) Phenanthrene-d10	17.017	188	7734	0.40	ng	0.00
29) Chrysene-d12	21.227	240	7630	0.40	ng	# 0.00
36) Perylene-d12	23.422	264	8663	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.243	112	2110	0.37	ng	0.00
5) Phenol-d6	6.813	99	2600	0.36	ng	0.00
8) Nitrobenzene-d5	8.780	82	2515	0.36	ng	0.00
11) 2-Methylnaphthalene-d10	12.002	152	3790	0.35	ng	0.00
14) 2,4,6-Tribromophenol	15.765	330	784	0.43	ng	0.00
15) 2-Fluorobiphenyl	12.885	172	4870	0.34	ng	0.00
27) Fluoranthene-d10	19.057	212	8002	0.35	ng	0.00
31) Terphenyl-d14	19.668	244	5900	0.34	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.213	88	1147	0.40	ng	89
3) n-Nitrosodimethylamine	3.527	42	1576	0.38	ng	98
6) bis(2-Chloroethyl)ether	7.071	93	2061	0.33	ng	96
9) Naphthalene	10.453	128	6693	0.34	ng	98
10) Hexachlorobutadiene	10.744	225	1310	0.41	ng	# 99
12) 2-Methylnaphthalene	12.078	142	4321	0.35	ng	95
16) Acenaphthylene	13.989	152	6197	0.34	ng	99
17) Acenaphthene	14.332	154	4016	0.32	ng	88
18) Fluorene	15.321	166	5069	0.34	ng	99
20) 4,6-Dinitro-2-methylph...	15.423	198	489	0.33	ng	# 22
21) 4-Bromophenyl-phenylether	16.226	248	1456	0.36	ng	# 88
22) Hexachlorobenzene	16.335	284	1820	0.38	ng	# 87
23) Atrazine	16.494	200	1406	0.36	ng	# 95
24) Pentachlorophenol	16.676	266	778	0.33	ng	98
25) Phenanthrene	17.066	178	7631	0.32	ng	99
26) Anthracene	17.151	178	6800	0.33	ng	98
28) Fluoranthene	19.092	202	8978	0.34	ng	# 97
30) Pyrene	19.454	202	9150	0.32	ng	100
32) Benzo(a)anthracene	21.206	228	8009	0.33	ng	97
33) Chrysene	21.259	228	9041	0.34	ng	98
34) Bis(2-ethylhexyl)phtha...	21.152	149	5924	0.34	ng	93
35) Indeno(1,2,3-cd)pyrene	25.620	276	12212	0.41	ng	98
37) Benzo(b)fluoranthene	22.765	252	8959	0.30	ng	# 86
38) Benzo(k)fluoranthene	22.810	252	10676m	0.33	ng	
39) Benzo(a)pyrene	23.330	252	8843	0.32	ng	# 82
40) Dibenzo(a,h)anthracene	25.630	278	9659	0.34	ng	# 86
41) Benzo(g,h,i)perylene	26.287	276	10536	0.35	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101220\
 Data File : BN012146.D
 Acq On : 12 Oct 2020 11:50
 Operator : CG/JU
 Sample : PB132270BS
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB132270BS

Manual Integrations
 APPROVED

mohammad
 10/13/2020 11:08:33 AM

Quant Time: Oct 12 12:19:11 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 12 11:15:56 2020
 Response via : Initial Calibration









#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.635 min Scan# 578
Delta R.T. 0.001 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 152 Resp: 1645
Ion Ratio Lower Upper
152 100
150 160.6 118.3 177.5
115 76.9 51.3 76.9

Instrument :
BNA_N
ClientSampled :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#2
1,4-Dioxane
Concen: 0.40 ng
RT: 3.213 min Scan# 29
Delta R.T. 0.008 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 88 Resp: 1147
Ion Ratio Lower Upper
88 100
58 65.6 63.3 94.9
43 39.3 33.0 49.4





#3
n-Nitrosodimethylamine
Concen: 0.38 ng
RT: 3.527 min Scan# 68
Delta R.T. 0.008 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50





Tgt Ion: 42 Resp: 1576

Ion	Ratio	Lower	Upper
42	100		
74	78.6	64.4	96.6
44	7.2	6.7	10.1

Instrument :
BNA_N
ClientSampled :
PB132270BS

Manual Integrations
APPROVED




mohammad
10/13/2020 11:08:33 AM



#4
2-Fluorophenol
Concen: 0.37 ng
RT: 5.243 min Scan# 281
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 112 Resp: 2110

Ion	Ratio	Lower	Upper
112	100		
64	68.1	49.0	73.6
63	43.6	31.8	47.6









#5
Phenol-d6
Concen: 0.36 ng
RT: 6.813 min Scan# 476
Delta R.T. 0.008 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 99 Resp: 2600
Ion Ratio Lower Upper
99 100
42 32.5 23.4 35.0
71 49.7 38.1 57.1

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#6
bis(2-Chloroethyl)ether
Concen: 0.33 ng
RT: 7.071 min Scan# 508
Delta R.T. 0.008 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50


Tgt Ion: 93 Resp: 2061
Ion Ratio Lower Upper
93 100
63 80.9 61.1 91.7
95 31.3 25.5 38.3





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.402 min Scan# 827
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50




Instrument :
BNA_N
ClientSampleId :
PB132270BS




Tgt Ion:136 Resp: 6779
Ion Ratio Lower Upper
136 100
137 12.3 9.5 14.3
54 11.6 5.6 8.4#
68 6.1 3.2 4.8#

Manual Integrations
APPROVED



mohammad
10/13/2020 11:08:33 AM




#8
Nitrobenzene-d5
Concen: 0.36 ng
RT: 8.780 min Scan# 699
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50



Tgt Ion: 82 Resp: 2515
Ion Ratio Lower Upper
82 100
128 37.8 34.2 51.2
54 60.9 43.1 64.7









#9
Naphthalene
Concen: 0.34 ng
RT: 10.453 min Scan# 831
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	128	Resp:	6693
Ion	Ratio	Lower	Upper
128	100		
129	12.2	9.7	14.5
127	15.2	11.0	16.4

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#10
Hexachlorobutadiene
Concen: 0.41 ng
RT: 10.744 min Scan# 854
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	225	Resp:	1310
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.1	51.9	77.9









#11
2-Methylnaphthalene-d10
Concen: 0.35 ng
RT: 12.002 min Scan# 1024
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:152 Resp: 3790
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#12
2-Methylnaphthalene
Concen: 0.35 ng
RT: 12.078 min Scan# 1041
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:142 Resp: 4321
Ion Ratio Lower Upper
142 100
141 89.8 70.0 105.0
115 51.7 35.8 53.6









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.268 min Scan# 1276
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:164 Resp: 3746
Ion Ratio Lower Upper
164 100
162 107.0 83.6 125.4
160 50.4 41.2 61.8

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#14
2,4,6-Tribromophenol
Concen: 0.43 ng
RT: 15.765 min Scan# 1394
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:330 Resp: 784
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 50.3 33.7 50.5









#15
2-Fluorobiphenyl
Concen: 0.34 ng
RT: 12.885 min Scan# 1167
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	172	Resp:	4870
Ion Ratio	Lower	Upper	
172	100		
171	36.9	27.4	41.2
170	25.8	17.8	26.6

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#16
Acenaphthylene
Concen: 0.34 ng
RT: 13.989 min Scan# 1254
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50


Tgt Ion:	152	Resp:	6197
Ion Ratio	Lower	Upper	
152	100		
151	19.2	15.9	23.9
153	13.0	10.5	15.7





#17
Acenaphthene
Concen: 0.32 ng
RT: 14.332 min Scan# 1281
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50




Instrument :
BNA_N
ClientSampleId :
PB132270BS



Tgt Ion:154 Resp: 4016
Ion Ratio Lower Upper
154 100
153 118.8 83.4 125.2
152 58.1 42.8 64.2




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#18
Fluorene
Concen: 0.34 ng
RT: 15.321 min Scan# 1359
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:166 Resp: 5069
Ion Ratio Lower Upper
166 100
165 97.7 78.8 118.2
167 13.9 11.2 16.8









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.017 min Scan# 1496
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:188 Resp: 7734
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 7.7 11.5

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM




#20
4,6-Dinitro-2-methylphenol
Concen: 0.33 ng
RT: 15.423 min Scan# 1367
Delta R.T. 0.013 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:198 Resp: 489
Ion Ratio Lower Upper
198 100
51 136.0 45.0 67.4#
105 57.3 30.4 45.6#









#21
4-Bromophenyl-phenylether
Concen: 0.36 ng
RT: 16.226 min Scan# 1431
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50





Tgt Ion:248 Resp: 1456
Ion Ratio Lower Upper
248 100
250 101.7 82.7 124.1
141 65.0 33.7 50.5#



#22
Hexachlorobenzene
Concen: 0.38 ng
RT: 16.335 min Scan# 1440
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50




Tgt Ion:284 Resp: 1820
Ion Ratio Lower Upper
284 100
142 53.4 32.4 48.6#
249 31.5 26.8 40.2



Instrument :
BNA_N
ClientSampled :
PB132270BS


Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM

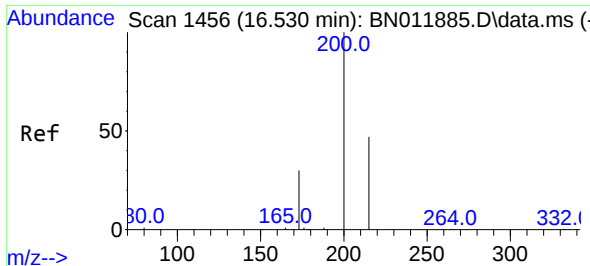

#23
Atrazine
Concen: 0.36 ng
RT: 16.494 min Scan# 1453
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50




Instrument :
BNA_N
ClientSampleId :
PB132270BS




Tgt Ion:200 Resp: 1406
Ion Ratio Lower Upper
200 100
173 30.0 18.7 28.1#
215 49.4 40.2 60.4

Manual Integrations
APPROVED



mohammad
10/13/2020 11:08:33 AM



#24
Pentachlorophenol
Concen: 0.33 ng
RT: 16.676 min Scan# 1468
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50



Tgt Ion:266 Resp: 778
Ion Ratio Lower Upper
266 100
264 63.0 51.2 76.8
268 64.1 52.4 78.6





#25
Phenanthrene
Concen: 0.32 ng
RT: 17.066 min Scan# 1500
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50





Tgt Ion:178 Resp: 7631

Ion	Ratio	Lower	Upper
178	100		
176	19.5	15.1	22.7
179	15.3	12.3	18.5

Instrument :
BNA_N
ClientSampled :
PB132270BS

Manual Integrations
APPROVED




mohammad
10/13/2020 11:08:33 AM



#26
Anthracene
Concen: 0.33 ng
RT: 17.151 min Scan# 1507
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:178 Resp: 6800

Ion	Ratio	Lower	Upper
178	100		
176	19.0	14.6	21.8
179	14.8	12.4	18.6









#27
Fluoranthene-d10
Concen: 0.35 ng
RT: 19.057 min Scan# 1788
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion	Ratio	Lower	Upper
212	100		
106	9.3	6.4	9.6
104	5.9	3.9	5.9#

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#28
Fluoranthene
Concen: 0.34 ng
RT: 19.092 min Scan# 1795
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion	Ratio	Lower	Upper
202	100		
101	8.6	5.4	8.2#
203	16.4	13.8	20.6









#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.227 min Scan# 2094
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:240 Resp: 7630
Ion Ratio Lower Upper
240 100
120 10.0 3.5 5.3#
236 27.2 20.5 30.7

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#30
Pyrene
Concen: 0.32 ng
RT: 19.454 min Scan# 1868
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50


Tgt Ion:202 Resp: 9150
Ion Ratio Lower Upper
202 100
200 20.8 16.5 24.7
203 17.4 13.9 20.9





#31
Terphenyl-d14
Concen: 0.34 ng
RT: 19.668 min Scan# 1911
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50




Instrument :
BNA_N
ClientSampleId :
PB132270BS




Tgt Ion:244 Resp: 5900
Ion Ratio Lower Upper
244 100
212 10.3 7.3 10.9
122 12.0 7.8 11.6#

Manual Integrations
APPROVED



mohammad
10/13/2020 11:08:33 AM



#32
Benzo(a)anthracene
Concen: 0.33 ng
RT: 21.206 min Scan# 2092
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50



Tgt Ion:228 Resp: 8009
Ion Ratio Lower Upper
228 100
226 28.7 21.0 31.4
229 20.6 16.0 24.0









#33
Chrysene
Concen: 0.34 ng
RT: 21.259 min Scan# 2097
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion	Ratio	Lower	Upper
228	100		
226	30.8	23.3	34.9
229	20.4	15.8	23.8

Instrument :
BNA_N
ClientSampleId :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#34
Bis(2-ethylhexyl)phthalate
Concen: 0.34 ng
RT: 21.152 min Scan# 2087
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion	Ratio	Lower	Upper
149	100		
167	25.0	23.6	35.4
279	4.5	4.0	6.0









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.620 min Scan# 3144
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 276 Resp: 12212
Ion Ratio Lower Upper
276 100
138 17.9 13.0 19.4
277 24.2 20.0 30.0

Instrument :
BNA_N
ClientSampled :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.422 min Scan# 2502
Delta R.T. -0.003 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion: 264 Resp: 8663
Ion Ratio Lower Upper
264 100
260 24.5 19.6 29.4
265 69.1 38.6 58.0#









#37
Benzo(b)fluoranthene
Concen: 0.30 ng
RT: 22.765 min Scan# 2310
Delta R.T. -0.003 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:252 Resp: 8959
Ion Ratio Lower Upper
252 100
253 29.9 19.1 28.7#
125 14.4 6.2 9.2#

Instrument :
BNA_N
ClientSampled :
PB132270BS




Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM



#38
Benzo(k)fluoranthene
Concen: 0.33 ng m
RT: 22.810 min Scan# 2323
Delta R.T. -0.003 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:252 Resp: 10676
Ion Ratio Lower Upper
252 100
253 29.8 19.3 28.9#
125 13.5 6.0 9.0#









#39
Benzo(a)pyrene
Concen: 0.32 ng
RT: 23.330 min Scan# 2475
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	252	Resp:	8843
Ion Ratio	Lower	Upper	
252	100		
253	32.8	19.8	29.6#
125	17.3	7.3	10.9#

Instrument :
BNA_N
ClientSampled :
PB132270BS




Manual Integrations
APPROVED


mohammad
10/13/2020 11:08:33 AM



#40
Dibenzo(a,h)anthracene
Concen: 0.34 ng
RT: 25.630 min Scan# 3147
Delta R.T. -0.003 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	278	Resp:	9659
Ion Ratio	Lower	Upper	
278	100		
139	16.0	8.6	13.0#
279	32.0	19.8	29.8#





#41
Benzo(g,h,i)perylene
Concen: 0.35 ng
RT: 26.287 min Scan# 3339
Delta R.T. 0.000 min
Lab File: BN012146.D
Acq: 12 Oct 2020 11:50

Tgt Ion:	276	Resp:	10536
Ion Ratio	Lower	Upper	
276	100		
277	26.3	19.4	29.0
138	19.1	11.3	16.9#

Instrument :
BNA_N
ClientSampleId :
PB132270BS

Manual Integrations
APPROVED

mohammad
10/13/2020 11:08:33 AM

