
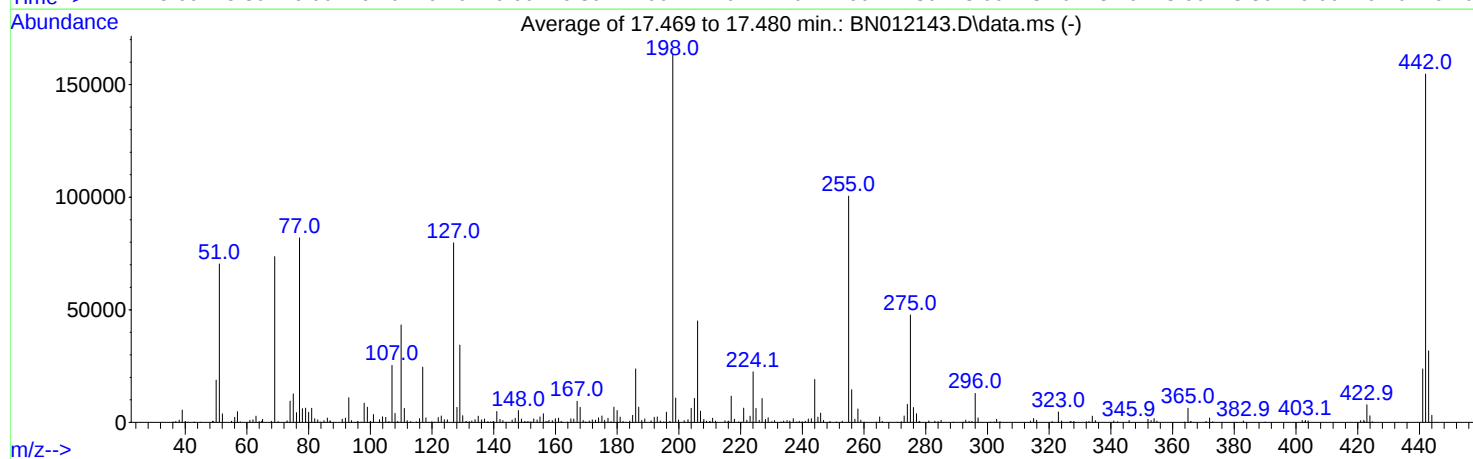


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101220\
Data File : BN012143.D
Acq On : 12 Oct 2020 09:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN092320.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Oct 12 11:15:56 2020

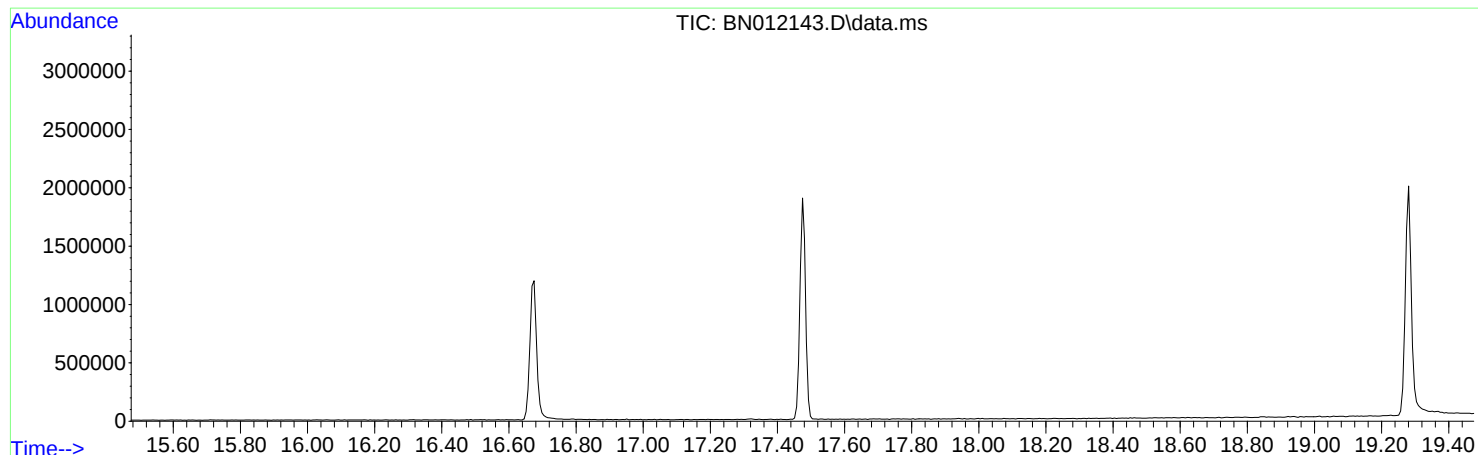

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	70355	PASS
68	69	0.00	2	0.7	497	PASS
69	198	0.00	100	45.1	73648	PASS
70	69	0.00	2	0.5	368	PASS
127	198	10	80	48.8	79725	PASS
197	198	0.00	2	0.3	516	PASS
198	198	100	100	100.0	163400	PASS
199	198	5	9	6.6	10834	PASS
275	198	10	60	29.2	47693	PASS
365	198	1	100	3.8	6274	PASS
441	198	0.01	100	14.5	23755	PASS
442	198	50	100	94.7	154701	PASS
443	442	15	24	20.5	31752	PASS