

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
 Data File : BN016887.D
 Acq On : 11 Oct 2021 18:32
 Operator : CG/JU
 Sample : SSTDICC0.2
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Quant Time: Oct 12 02:17:28 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 12 02:08:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	18617	0.400	ng	0.00
7) Naphthalene-d8	10.457	136	85068	0.400	ng	0.00
13) Acenaphthene-d10	14.294	164	45093	0.400	ng	0.00
19) Phenanthrene-d10	17.042	188	83299	0.400	ng	0.00
29) Chrysene-d12	21.227	240	81325	0.400	ng	#-0.01
35) Perylene-d12	23.478	264	85531	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	9951	0.214	ng	0.00
5) Phenol-d6	6.868	99	10845	0.205	ng	0.00
8) Nitrobenzene-d5	8.835	82	10624	0.178	ng	0.00
11) 2-Methylnaphthalene-d10	12.043	152	25360	0.200	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	3692	0.158	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	35853	0.197	ng	0.00
27) Fluoranthene-d10	19.073	212	44243	0.191	ng	0.00
31) Terphenyl-d14	19.683	244	37745	0.213	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.281	88	2922	0.351	ng	# 65
3) n-Nitrosodimethylamine	3.613	42	2987	0.204	ng	98
6) bis(2-Chloroethyl)ether	7.126	93	11057	0.215	ng	100
9) Naphthalene	10.495	128	49216	0.212	ng	100
10) Hexachlorobutadiene	10.787	225	9064	0.205	ng	# 99
12) 2-Methylnaphthalene	12.114	142	30330	0.205	ng	99
16) Acenaphthylene	14.015	152	35941	0.181	ng	100
17) Acenaphthene	14.357	154	25854	0.195	ng	99
18) Fluorene	15.347	166	31159	0.194	ng	100
20) 4,6-Dinitro-2-methylph...	15.436	198	1462	0.105	ng	# 90
21) 4-Bromophenyl-phenylether	16.239	248	9765	0.188	ng	97
22) Hexachlorobenzene	16.348	284	11624	0.196	ng	99
23) Atrazine	16.518	200	6308	0.153	ng	99
24) Pentachlorophenol	16.701	266	2893	0.149	ng	99
25) Phenanthrene	17.078	178	49494	0.200	ng	100
26) Anthracene	17.163	178	40454	0.184	ng	100
28) Fluoranthene	19.103	202	54228	0.195	ng	100
30) Pyrene	19.465	202	54609	0.218	ng	100
32) Benzo(a)anthracene	21.217	228	51520	0.205	ng	99
33) Chrysene	21.270	228	56527	0.221	ng	100
34) Bis(2-ethylhexyl)phtha...	21.164	149	23339	0.183	ng	100
36) Indeno(1,2,3-cd)pyrene	25.750	276	68646	0.212	ng	99
37) Benzo(b)fluoranthene	22.803	252	57282	0.212	ng	98
38) Benzo(k)fluoranthene	22.848	252	58735	0.223	ng	97
39) Benzo(a)pyrene	23.378	252	51854	0.210	ng	97
40) Dibenzo(a,h)anthracene	25.771	278	55619	0.210	ng	98
41) Benzo(g,h,i)perylene	26.438	276	59108	0.210	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016887.D
Acq On : 11 Oct 2021 18:32
Operator : CG/JU
Sample : SSTDICC0.2
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2

Quant Time: Oct 12 02:17:28 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 02:08:51 2021
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.688 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:152 Resp: 18617
 Ion Ratio Lower Upper
 152 100
 150 154.6 124.2 186.4
 115 58.7 47.0 70.6



#2
 1,4-Dioxane
 Concen: 0.351 ng
 RT: 3.281 min Scan# 22
 Delta R.T. -0.009 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Tgt Ion: 88 Resp: 2922
 Ion Ratio Lower Upper
 88 100
 43 98.6 32.0 48.0#
 58 78.3 60.6 90.8









#3
 n-Nitrosodimethylamine
 Concen: 0.204 ng
 RT: 3.613 min Scan# 58
 Delta R.T. -0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion: 42 Resp: 2987




Ion	Ratio	Lower	Upper
42	100		
74	148.9	117.2	175.8
44	6.9	5.4	8.0




#4
 2-Fluorophenol
 Concen: 0.214 ng
 RT: 5.300 min Scan# 241
 Delta R.T. -0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Tgt Ion: 112 Resp: 9951

Ion	Ratio	Lower	Upper
112	100		
64	55.4	44.5	66.7
63	28.0	22.1	33.1









#5
Phenol-d6
Concen: 0.205 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion: 99 Resp: 10845
Ion Ratio Lower Upper
99 100
42 17.2 13.9 20.9
71 30.5 24.5 36.7



#6
bis(2-Chloroethyl)ether
Concen: 0.215 ng
RT: 7.126 min Scan# 439
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion: 93 Resp: 11057
Ion Ratio Lower Upper
93 100
63 75.1 59.8 89.6
95 32.9 26.4 39.6









#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.457 min Scan# 737
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:	136	Resp:	85068
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.8	13.2
54	4.9	3.8	5.6
68	4.2	3.4	5.0



#8
Nitrobenzene-d5
Concen: 0.178 ng
RT: 8.835 min Scan# 609
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:	82	Resp:	10624
Ion Ratio	Lower	Upper	
82	100		
128	47.7	37.8	56.6
54	44.7	35.3	52.9









#9
Naphthalene
Concen: 0.212 ng
RT: 10.495 min Scan# 740
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:128 Resp: 49216
Ion Ratio Lower Upper
128 100
129 11.0 8.8 13.2
127 13.5 10.7 16.1



#10
Hexachlorobutadiene
Concen: 0.205 ng
RT: 10.787 min Scan# 763
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:225 Resp: 9064
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.6 50.9 76.3







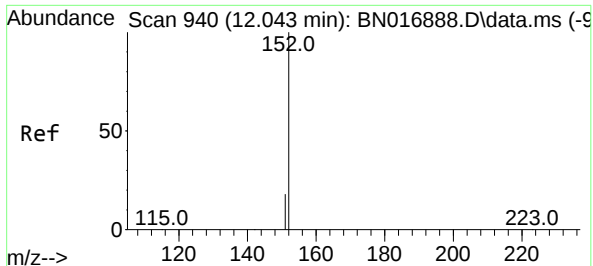

#11
2-Methylnaphthalene-d10
Concen: 0.200 ng
RT: 12.043 min Scan# 940
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:152 Resp: 25360
Ion Ratio Lower Upper
152 100
151 20.2 16.3 24.5

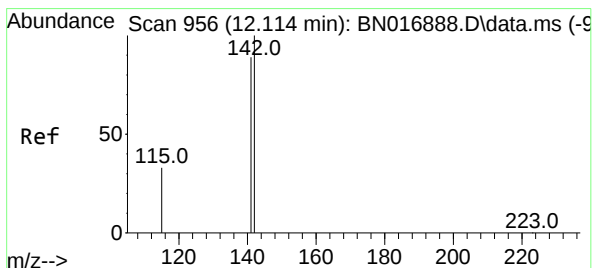

#12
2-Methylnaphthalene
Concen: 0.205 ng
RT: 12.114 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:142 Resp: 30330
Ion Ratio Lower Upper
142 100
141 89.5 71.0 106.4
115 33.9 26.6 40.0









#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.294 min Scan# 1185
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:164 Resp: 45093
Ion Ratio Lower Upper
164 100
162 102.0 81.8 122.8
160 45.9 37.0 55.4



#14
2,4,6-Tribromophenol
Concen: 0.158 ng
RT: 15.791 min Scan# 1303
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:330 Resp: 3692
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 30.6 24.3 36.5









#15
2-Fluorobiphenyl
Concen: 0.197 ng
RT: 12.924 min Scan# 1077
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:172 Resp: 35853
Ion Ratio Lower Upper
172 100
171 34.8 27.7 41.5
170 23.2 18.3 27.5



#16
Acenaphthylene
Concen: 0.181 ng
RT: 14.015 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:152 Resp: 35941
Ion Ratio Lower Upper
152 100
151 19.4 15.5 23.3
153 13.1 10.4 15.6









#17
Acenaphthene
Concen: 0.195 ng
RT: 14.357 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:154 Resp: 25854
Ion Ratio Lower Upper
154 100
153 113.8 90.6 135.8
152 55.0 43.7 65.5



#18
Fluorene
Concen: 0.194 ng
RT: 15.347 min Scan# 1268
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:166 Resp: 31159
Ion Ratio Lower Upper
166 100
165 97.5 78.2 117.2
167 13.3 10.8 16.2







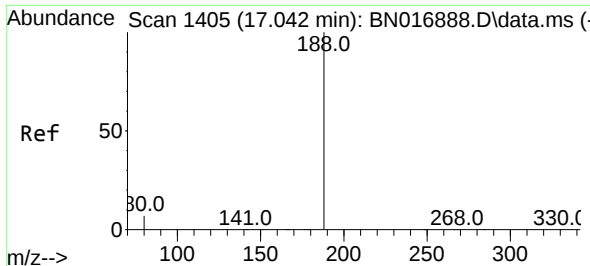

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:188 Resp: 83299
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.0 5.4 8.2

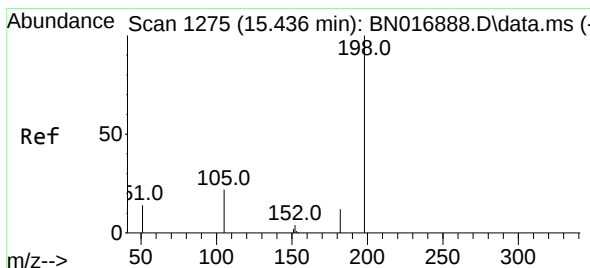

#20
4,6-Dinitro-2-methylphenol
Concen: 0.105 ng
RT: 15.436 min Scan# 1275
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:198 Resp: 1462
Ion Ratio Lower Upper
198 100
182 17.9 11.1 16.7#
77 0.0 0.0 0.0









#21
4-Bromophenyl-phenylether
Concen: 0.188 ng
RT: 16.239 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:248 Resp: 9765
Ion Ratio Lower Upper
248 100
250 95.7 75.8 113.6
141 63.8 47.4 71.2



#22
Hexachlorobenzene
Concen: 0.196 ng
RT: 16.348 min Scan# 1348
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:284 Resp: 11624
Ion Ratio Lower Upper
284 100
142 32.1 25.1 37.7
249 29.2 23.0 34.4









#23
 Atrazine
 Concen: 0.153 ng
 RT: 16.518 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:200 Resp: 6308
 Ion Ratio Lower Upper
 200 100
 173 25.1 19.7 29.5
 215 50.0 39.5 59.3



#24
 Pentachlorophenol
 Concen: 0.149 ng
 RT: 16.701 min Scan# 1377
 Delta R.T. 0.012 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Tgt Ion:266 Resp: 2893
 Ion Ratio Lower Upper
 266 100
 264 62.4 50.6 76.0
 268 63.7 51.3 76.9









#25
Phenanthrene
Concen: 0.200 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.2


Tgt Ion:178 Resp: 49494
Ion Ratio Lower Upper
178 100
176 18.9 15.0 22.6
179 15.7 12.3 18.5



#26
Anthracene
Concen: 0.184 ng
RT: 17.163 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:178 Resp: 40454
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.1 12.2 18.4







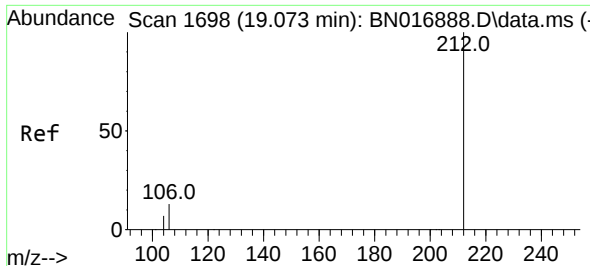

#27
Fluoranthene-d10
Concen: 0.191 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:212 Resp: 44243
Ion Ratio Lower Upper
212 100
106 13.4 10.8 16.2
104 7.4 5.9 8.9

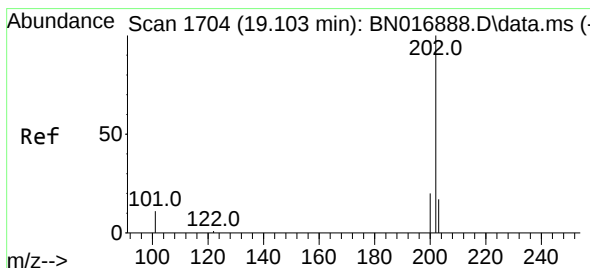

#28
Fluoranthene
Concen: 0.195 ng
RT: 19.103 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:202 Resp: 54228
Ion Ratio Lower Upper
202 100
101 11.3 9.0 13.6
203 17.2 13.8 20.8









#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.227 min Scan# 20
Delta R.T. -0.011 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:240 Resp: 81325
Ion Ratio Lower Upper
240 100
120 14.2 4.1 6.1#
236 26.6 20.1 30.1



#30
Pyrene
Concen: 0.218 ng
RT: 19.465 min Scan# 1777
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:202 Resp: 54609
Ion Ratio Lower Upper
202 100
200 20.5 16.4 24.6
203 17.4 14.0 21.0









#31
 Terphenyl-d14
 Concen: 0.213 ng
 RT: 19.683 min Scan# 1821
 Delta R.T. -0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2


Tgt Ion:244 Resp: 37745
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.5 8.3
 122 11.2 8.6 13.0



#32
 Benzo(a)anthracene
 Concen: 0.205 ng
 RT: 21.217 min Scan# 2000
 Delta R.T. -0.000 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Tgt Ion:228 Resp: 51520
 Ion Ratio Lower Upper
 228 100
 226 26.2 21.2 31.8
 229 19.9 15.8 23.6



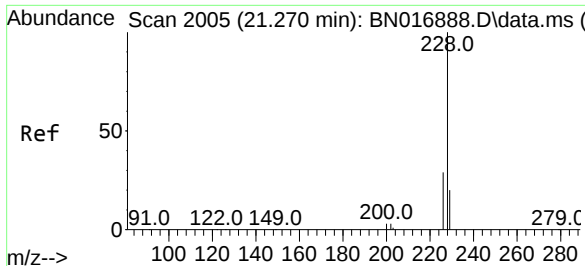

#33

Chrysene

Concen: 0.221 ng

RT: 21.270 min Scan# 2005

Delta R.T. -0.000 min

Lab File: BN016887.D

Acq: 11 Oct 2021 18:32

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.2





Tgt Ion:228 Resp: 56527

Ion Ratio Lower Upper

228 100

226 29.0 23.3 34.9

229 19.9 15.8 23.6



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.183 ng

RT: 21.164 min Scan# 1995

Delta R.T. -0.000 min

Lab File: BN016887.D

Acq: 11 Oct 2021 18:32




Tgt Ion:149 Resp: 23339


Ion Ratio Lower Upper

149 100

167 27.9 22.2 33.2


279 4.4 3.5 5.3








#35
Perylene-d12
Concen: 0.400 ng
RT: 23.478 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2







Tgt Ion:264 Resp: 85531
Ion Ratio Lower Upper
264 100
260 24.3 19.4 29.2
265 24.7 19.2 28.8



#36
Indeno(1,2,3-cd)pyrene
Concen: 0.212 ng
RT: 25.750 min Scan# 3089
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:276 Resp: 68646
Ion Ratio Lower Upper
276 100
138 26.5 20.1 30.1
277 25.1 20.1 30.1









#37
Benzo(b)fluoranthene
Concen: 0.212 ng
RT: 22.803 min Scan# 211
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2


Tgt Ion:252 Resp: 57282
Ion Ratio Lower Upper
252 100
253 23.1 17.8 26.8
125 10.7 8.1 12.1



#38
Benzo(k)fluoranthene
Concen: 0.223 ng
RT: 22.848 min Scan# 2241
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32


Tgt Ion:252 Resp: 58735
Ion Ratio Lower Upper
252 100
253 23.4 18.0 27.0
125 13.5 9.0 13.6








#39
Benzo(a)pyrene
Concen: 0.210 ng
RT: 23.378 min Scan# 2396
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.2







Tgt Ion:252 Resp: 51854
Ion Ratio Lower Upper
252 100
253 23.6 17.8 26.8
125 12.5 9.0 13.6



#40
Dibenzo(a,h)anthracene
Concen: 0.210 ng
RT: 25.771 min Scan# 3095
Delta R.T. -0.000 min
Lab File: BN016887.D
Acq: 11 Oct 2021 18:32

Tgt Ion:278 Resp: 55619
Ion Ratio Lower Upper
278 100
139 18.4 13.4 20.0
279 24.4 19.2 28.8





#41
 Benzo(g,h,i)perylene
 Concen: 0.210 ng
 RT: 26.438 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN016887.D
 Acq: 11 Oct 2021 18:32

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.2

Tgt Ion:	276	Resp:	59108
Ion Ratio	Lower	Upper	
276	100		
277	23.9	19.0	28.6
138	21.4	16.7	25.1

