

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
 Data File : BN016892.D
 Acq On : 11 Oct 2021 21:34
 Operator : CG/JU
 Sample : SSTDICC5.0
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Quant Time: Oct 12 02:18:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 12 02:08:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	24365	0.400	ng	0.00
7) Naphthalene-d8	10.457	136	99588	0.400	ng	0.00
13) Acenaphthene-d10	14.294	164	54097	0.400	ng	0.00
19) Phenanthrene-d10	17.042	188	103120	0.400	ng	0.00
29) Chrysene-d12	21.227	240	98570	0.400	ng	#-0.01
35) Perylene-d12	23.478	264	106176	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.291	112	275827	4.532	ng	0.00
5) Phenol-d6	6.868	99	321500	4.645	ng	0.00
8) Nitrobenzene-d5	8.822	82	359720	5.157	ng	-0.01
11) 2-Methylnaphthalene-d10	12.038	152	667509	4.501	ng	0.00
14) 2,4,6-Tribromophenol	15.791	330	152576	5.452	ng	0.00
15) 2-Fluorobiphenyl	12.924	172	940775	4.310	ng	0.00
27) Fluoranthene-d10	19.073	212	1277858	4.461	ng	0.00
31) Terphenyl-d14	19.683	244	1066579	4.962	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.281	88	82995	7.607	ng	# 92
3) n-Nitrosodimethylamine	3.604	42	96732	5.060	ng	97
6) bis(2-Chloroethyl)ether	7.126	93	297086	4.412	ng	98
9) Naphthalene	10.495	128	1189768	4.386	ng	100
10) Hexachlorobutadiene	10.787	225	231952	4.475	ng	# 99
12) 2-Methylnaphthalene	12.114	142	756333	4.358	ng	99
16) Acenaphthylene	14.015	152	1146545	4.803	ng	100
17) Acenaphthene	14.357	154	706738	4.454	ng	98
18) Fluorene	15.347	166	871219	4.516	ng	99
20) 4,6-Dinitro-2-methylph...	15.436	198	132103	7.646	ng	# 77
21) 4-Bromophenyl-phenylether	16.239	248	303642	4.724	ng	98
22) Hexachlorobenzene	16.348	284	322818	4.401	ng	99
23) Atrazine	16.519	200	252032	4.939	ng	98
24) Pentachlorophenol	16.689	266	177504	7.362	ng	99
25) Phenanthrene	17.078	178	1334858	4.359	ng	100
26) Anthracene	17.163	178	1268387	4.661	ng	100
28) Fluoranthene	19.103	202	1451044	4.219	ng	99
30) Pyrene	19.465	202	1530286	5.049	ng	100
32) Benzo(a)anthracene	21.217	228	1526709	5.008	ng	99
33) Chrysene	21.270	228	1471399	4.739	ng	99
34) Bis(2-ethylhexyl)phtha...	21.164	149	1024101	6.611	ng	99
36) Indeno(1,2,3-cd)pyrene	25.750	276	1871447	4.654	ng	99
37) Benzo(b)fluoranthene	22.800	252	1617155	4.812	ng	100
38) Benzo(k)fluoranthene	22.848	252	1559175	4.772	ng	98
39) Benzo(a)pyrene	23.378	252	1502200	4.892	ng	99
40) Dibenzo(a,h)anthracene	25.771	278	1547921	4.703	ng	99
41) Benzo(g,h,i)perylene	26.445	276	1621354	4.637	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016892.D
Acq On : 11 Oct 2021 21:34
Operator : CG/JU
Sample : SSTDICC5.0
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Quant Time: Oct 12 02:18:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 02:08:51 2021
Response via : Initial Calibration

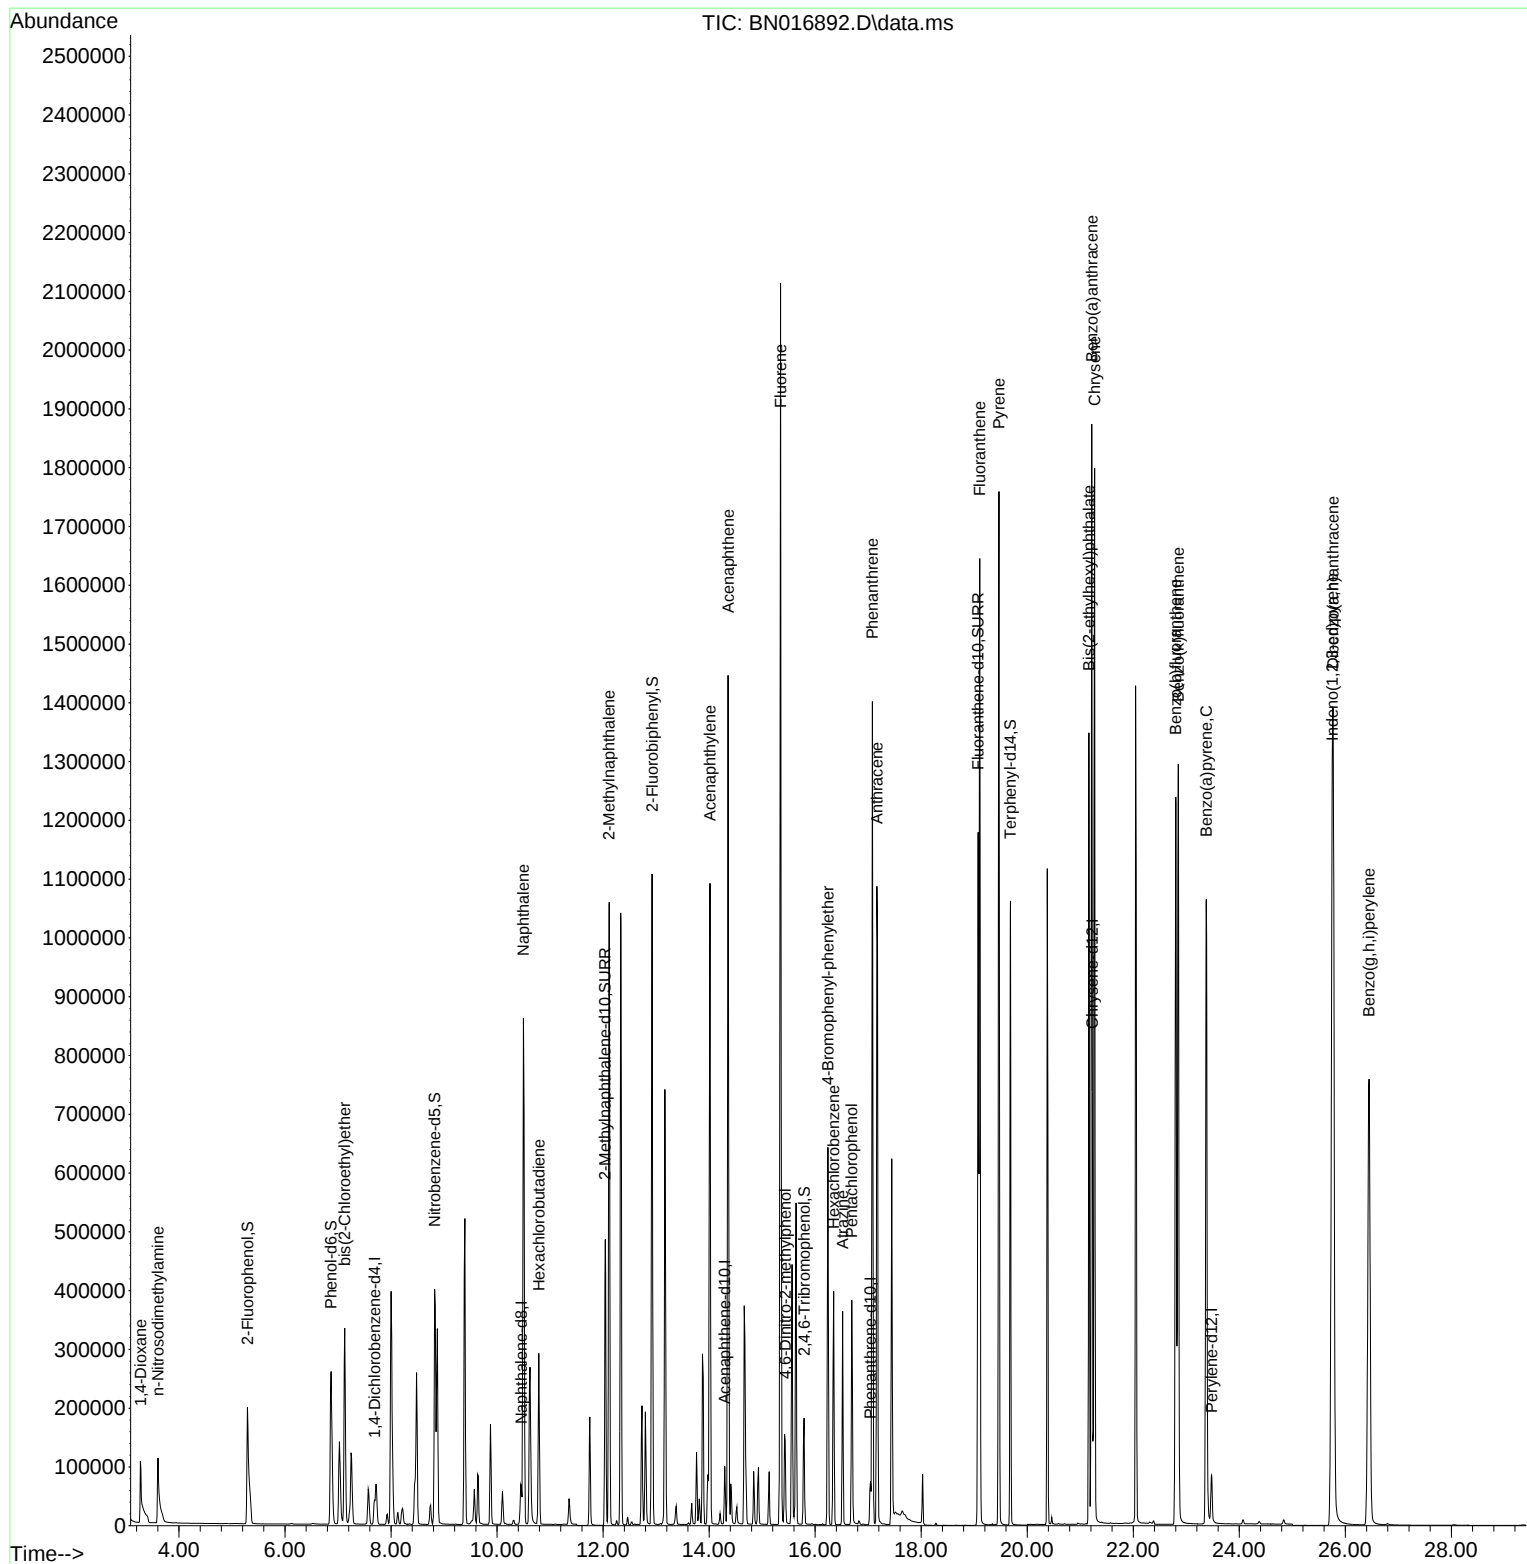






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.688 min Scan# 50
 Delta R.T. 0.000 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0







Tgt Ion:152 Resp: 24365
 Ion Ratio Lower Upper
 152 100
 150 155.7 124.2 186.4
 115 58.1 47.0 70.6

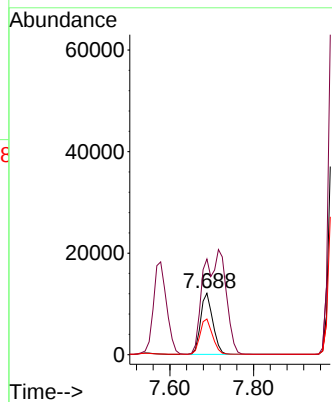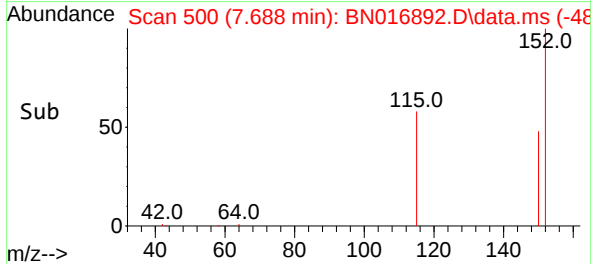

#2
 1,4-Dioxane
 Concen: 7.607 ng
 RT: 3.281 min Scan# 22
 Delta R.T. -0.009 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Tgt Ion: 88 Resp: 82995
 Ion Ratio Lower Upper
 88 100
 43 27.8 32.0 48.0#
 58 74.1 60.6 90.8



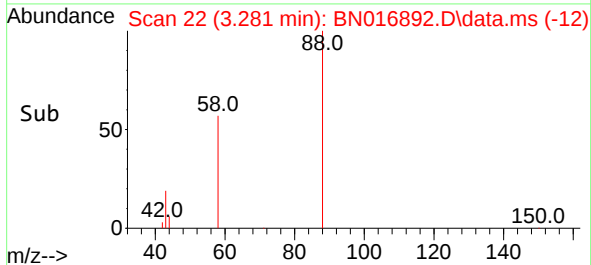





#3
 n-Nitrosodimethylamine
 Concen: 5.060 ng
 RT: 3.604 min Scan# 51
 Delta R.T. -0.009 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion: 42 Resp: 96732
 Ion Ratio Lower Upper
 42 100
 74 149.7 117.2 175.8
 44 5.6 5.4 8.0

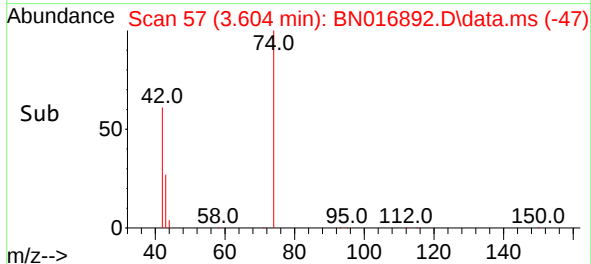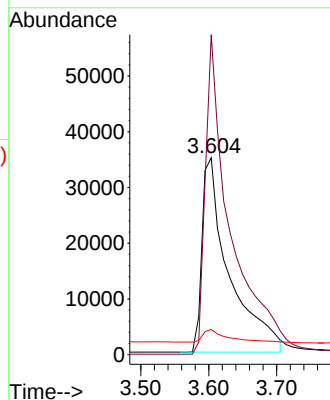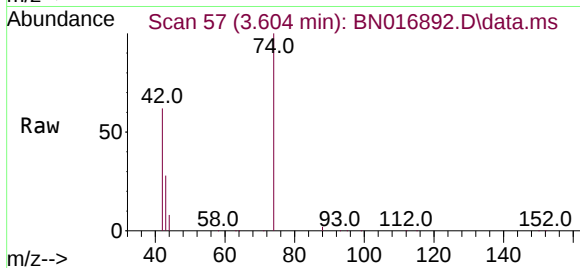

#4
 2-Fluorophenol
 Concen: 4.532 ng
 RT: 5.291 min Scan# 240
 Delta R.T. -0.009 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Tgt Ion: 112 Resp: 275827
 Ion Ratio Lower Upper
 112 100
 64 55.8 44.5 66.7
 63 28.0 22.1 33.1



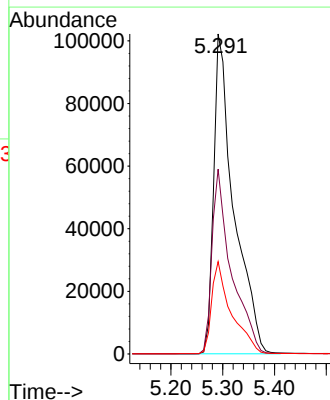
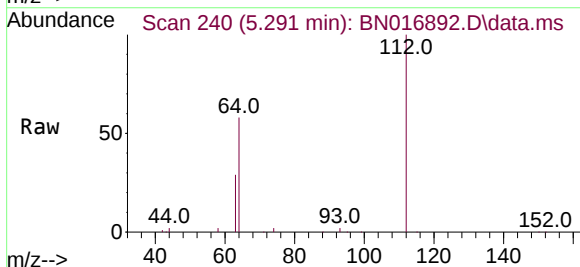




#5
Phenol-d6
Concen: 4.645 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion: 99 Resp: 321500
Ion Ratio Lower Upper
99 100
42 17.2 13.9 20.9
71 30.4 24.5 36.7

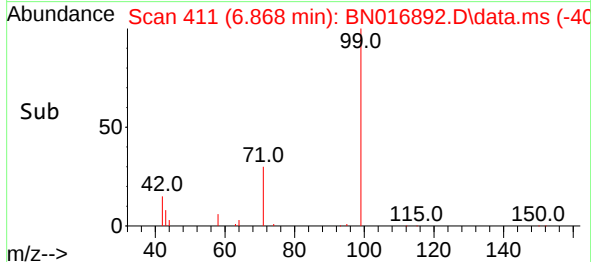

#6
bis(2-Chloroethyl)ether
Concen: 4.412 ng
RT: 7.126 min Scan# 439
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion: 93 Resp: 297086
Ion Ratio Lower Upper
93 100
63 72.6 59.8 89.6
95 32.1 26.4 39.6


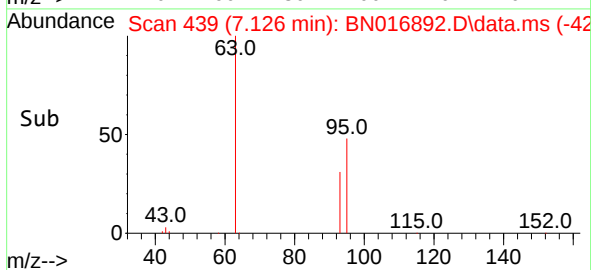

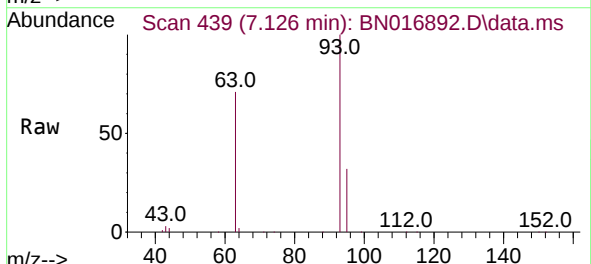




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.457 min Scan# 71
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:	136	Resp:	99588
Ion Ratio	Lower	Upper	
136	100		
137	11.0	8.8	13.2
54	4.6	3.8	5.6
68	4.1	3.4	5.0

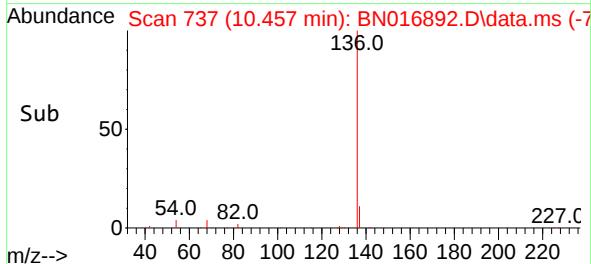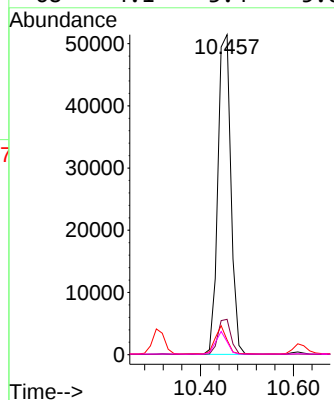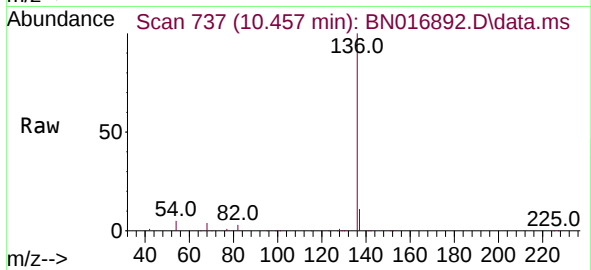

#8
Nitrobenzene-d5
Concen: 5.157 ng
RT: 8.822 min Scan# 608
Delta R.T. -0.013 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:	82	Resp:	359720
Ion Ratio	Lower	Upper	
82	100		
128	37.4	37.8	56.6#
54	52.1	35.3	52.9


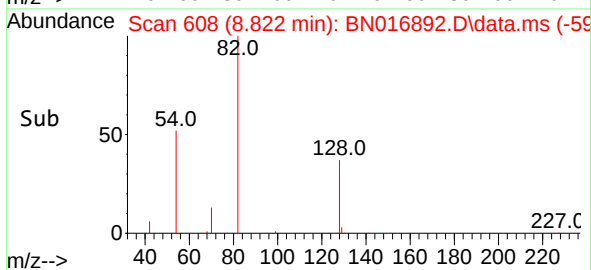
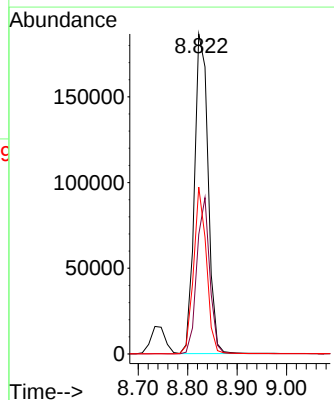





#9
Naphthalene
Concen: 4.386 ng
RT: 10.495 min Scan# 740
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:128 Resp: 1189768
Ion Ratio Lower Upper
128 100
129 11.1 8.8 13.2
127 13.2 10.7 16.1

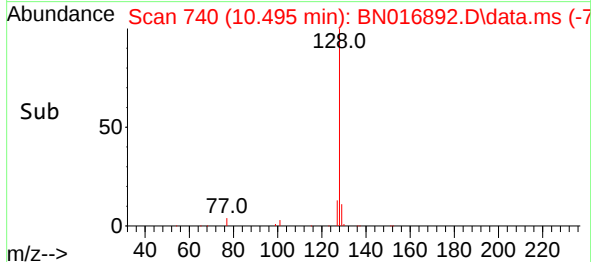

#10
Hexachlorobutadiene
Concen: 4.475 ng
RT: 10.787 min Scan# 763
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:225 Resp: 231952
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 50.9 76.3







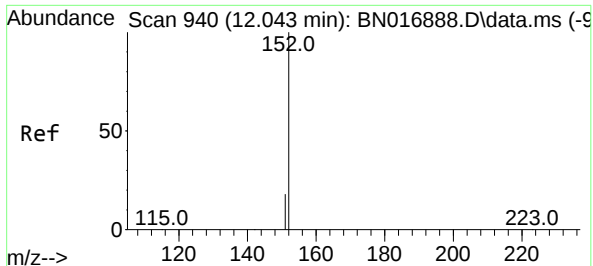

#11
2-Methylnaphthalene-d10
Concen: 4.501 ng
RT: 12.038 min Scan# 911
Delta R.T. -0.005 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:152 Resp: 667509
Ion Ratio Lower Upper
152 100
151 20.2 16.3 24.5

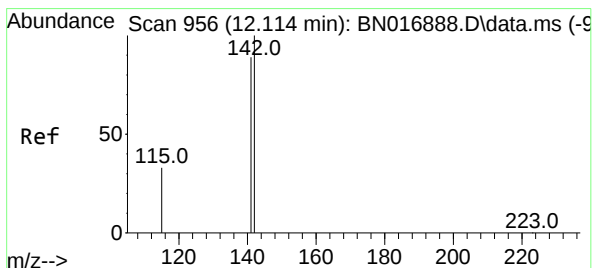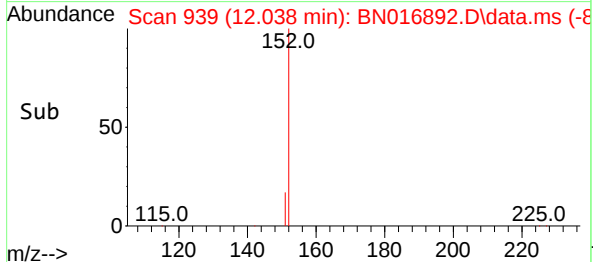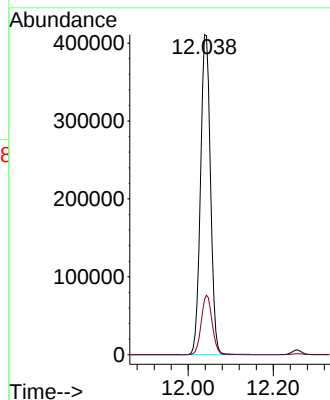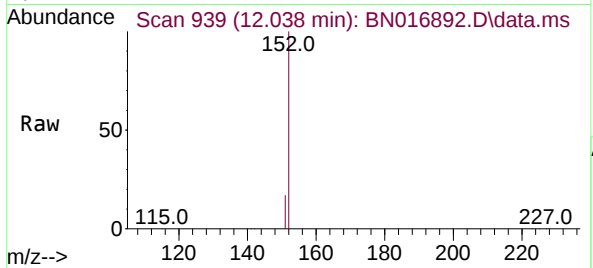

#12
2-Methylnaphthalene
Concen: 4.358 ng
RT: 12.114 min Scan# 956
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:142 Resp: 756333
Ion Ratio Lower Upper
142 100
141 87.7 71.0 106.4
115 32.6 26.6 40.0


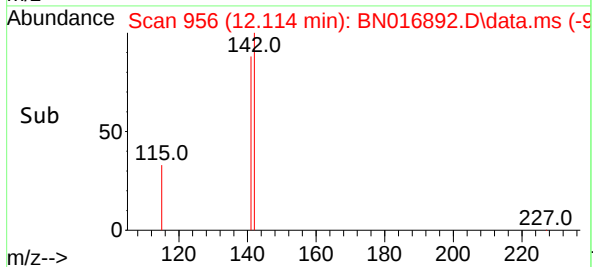
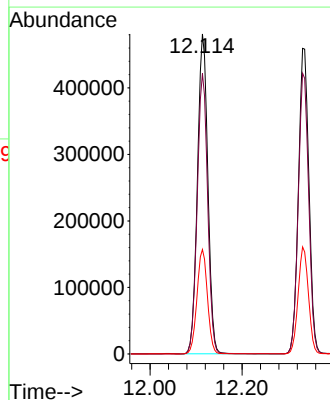
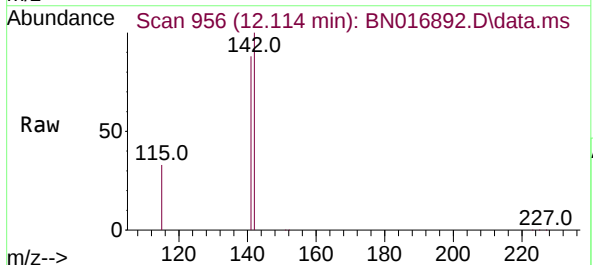




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.294 min Scan# 1185
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:164 Resp: 54097
Ion Ratio Lower Upper
164 100
162 102.2 81.8 122.8
160 45.9 37.0 55.4

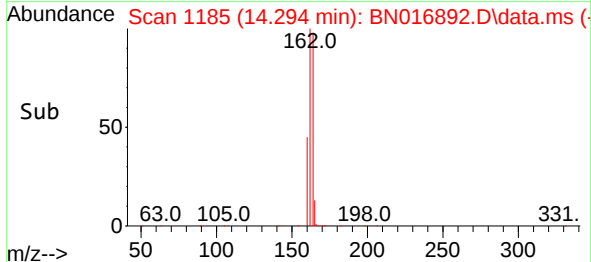

#14
2,4,6-Tribromophenol
Concen: 5.452 ng
RT: 15.791 min Scan# 1303
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:330 Resp: 152576
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 29.6 24.3 36.5


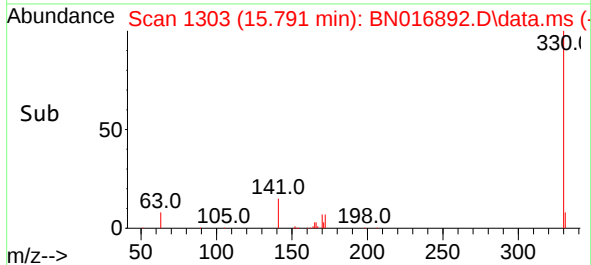




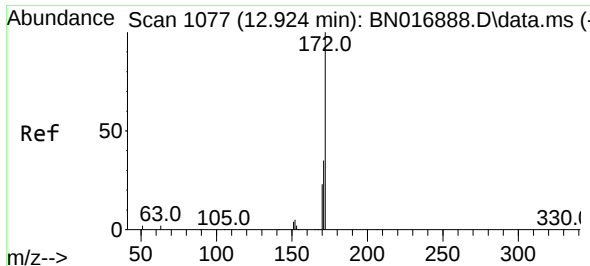

#15
2-Fluorobiphenyl
Concen: 4.310 ng
RT: 12.924 min Scan# 1077
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:172 Resp: 940775
Ion Ratio Lower Upper
172 100
171 34.3 27.7 41.5
170 22.7 18.3 27.5

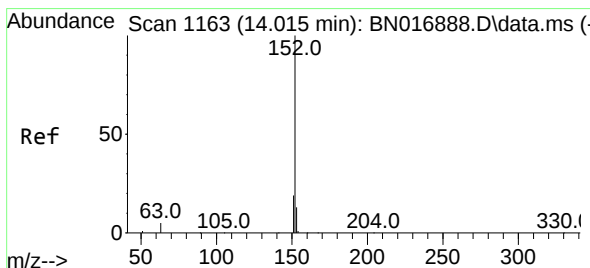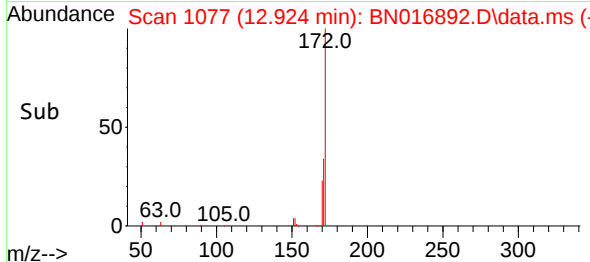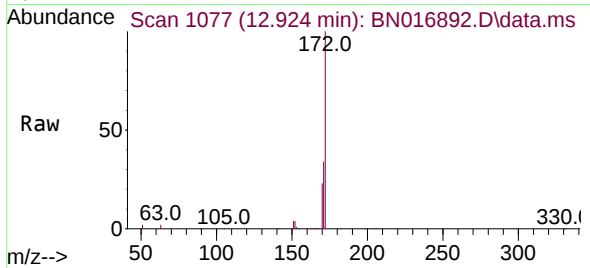

#16
Acenaphthylene
Concen: 4.803 ng
RT: 14.015 min Scan# 1163
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:152 Resp: 1146545
Ion Ratio Lower Upper
152 100
151 19.5 15.5 23.3
153 13.3 10.4 15.6


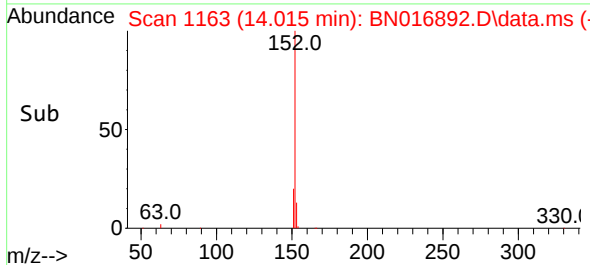

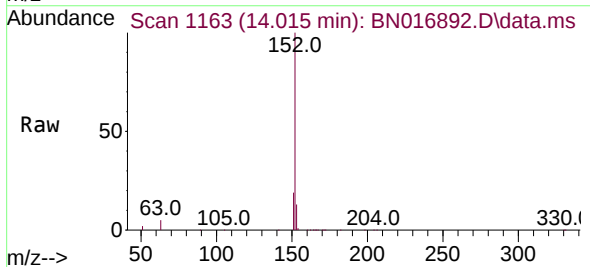




#17
Acenaphthene
Concen: 4.454 ng
RT: 14.357 min Scan# 1190
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:154 Resp: 706738
Ion Ratio Lower Upper
154 100
153 111.2 90.6 135.8
152 52.6 43.7 65.5

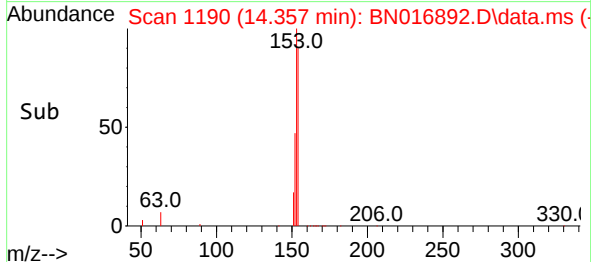

#18
Fluorene
Concen: 4.516 ng
RT: 15.347 min Scan# 1268
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:166 Resp: 871219
Ion Ratio Lower Upper
166 100
165 96.6 78.2 117.2
167 13.6 10.8 16.2




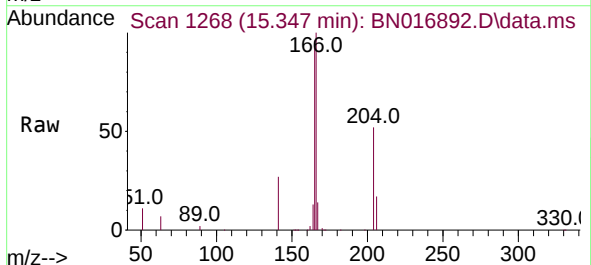


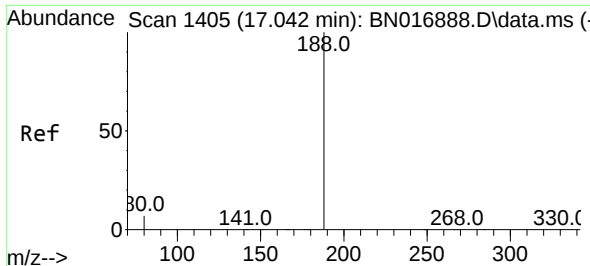

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.042 min Scan# 1405
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:188 Resp: 103120
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 6.8 5.4 8.2

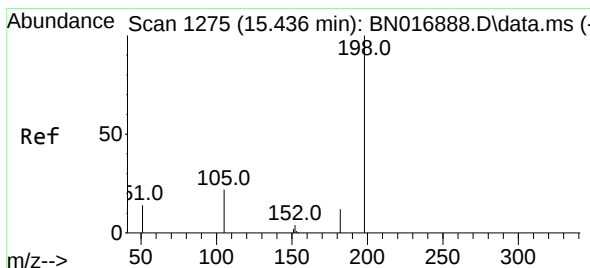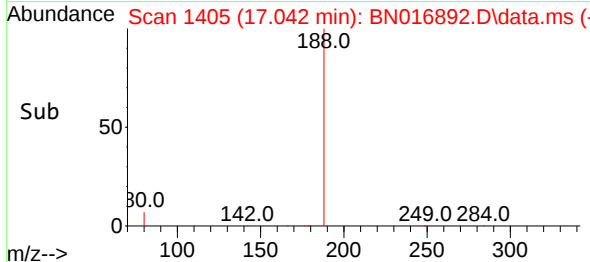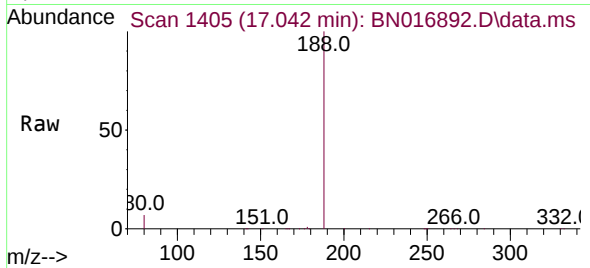

#20
4,6-Dinitro-2-methylphenol
Concen: 7.646 ng
RT: 15.436 min Scan# 1275
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:198 Resp: 132103
Ion Ratio Lower Upper
198 100
182 4.7 11.1 16.7#
77 0.0 0.0 0.0


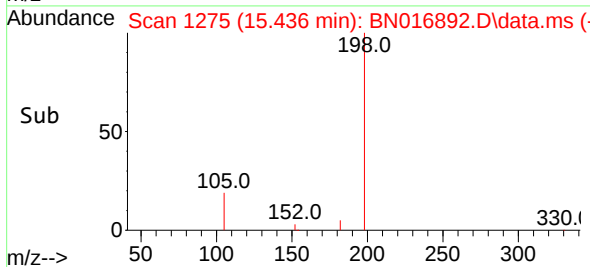

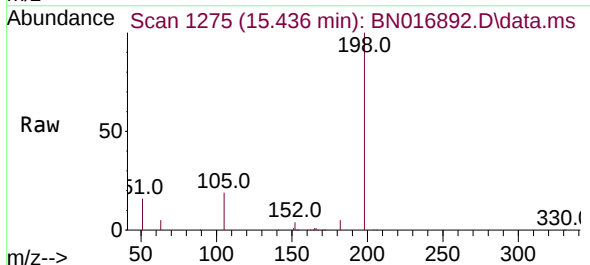




#21
4-Bromophenyl-phenylether
Concen: 4.724 ng
RT: 16.239 min Scan# 1339
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:248 Resp: 303642
Ion Ratio Lower Upper
248 100
250 94.9 75.8 113.6
141 55.1 47.4 71.2

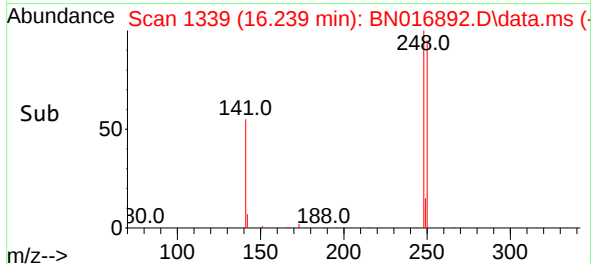

#22
Hexachlorobenzene
Concen: 4.401 ng
RT: 16.348 min Scan# 1348
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:284 Resp: 322818
Ion Ratio Lower Upper
284 100
142 31.9 25.1 37.7
249 29.2 23.0 34.4


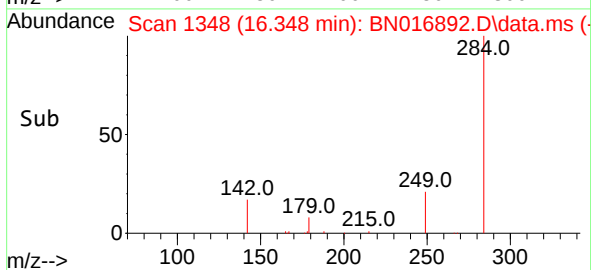

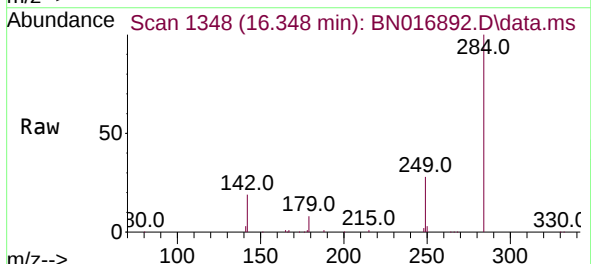




#23
 Atrazine
 Concen: 4.939 ng
 RT: 16.519 min Scan# 1362
 Delta R.T. -0.000 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:200 Resp: 252032
 Ion Ratio Lower Upper
 200 100
 173 26.5 19.7 29.5
 215 48.9 39.5 59.3

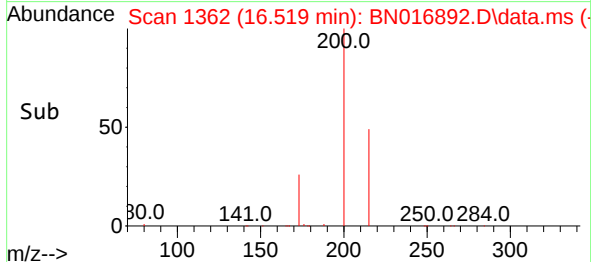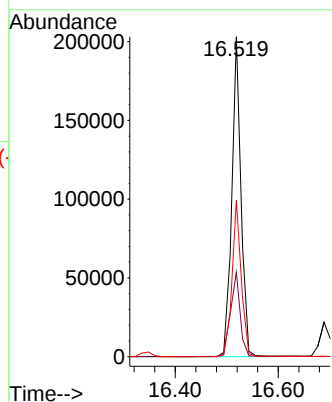

#24
 Pentachlorophenol
 Concen: 7.362 ng
 RT: 16.689 min Scan# 1376
 Delta R.T. -0.000 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Tgt Ion:266 Resp: 177504
 Ion Ratio Lower Upper
 266 100
 264 62.4 50.6 76.0
 268 64.0 51.3 76.9




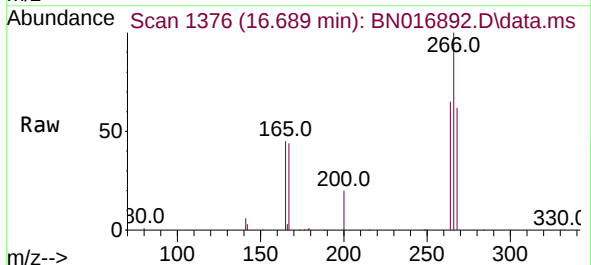


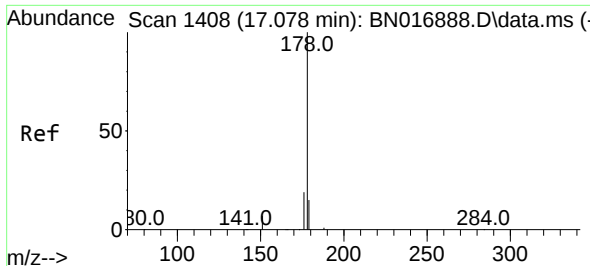

#25
Phenanthrene
Concen: 4.359 ng
RT: 17.078 min Scan# 1408
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:178 Resp: 1334858
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.5 12.3 18.5

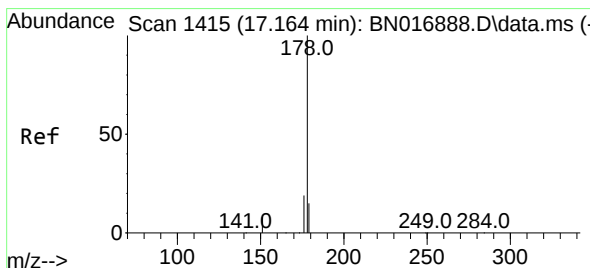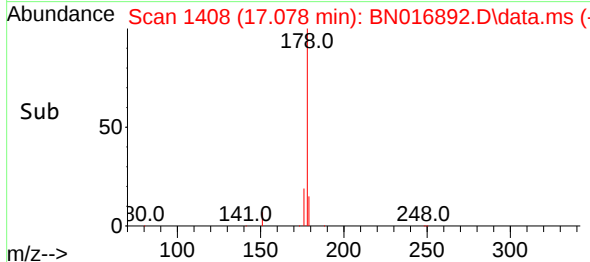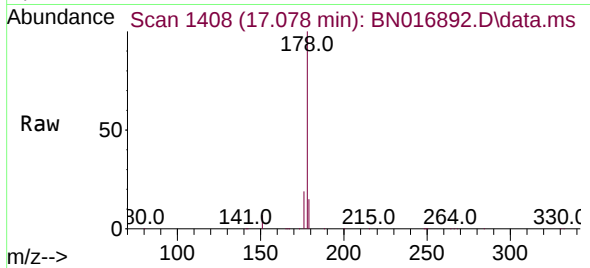

#26
Anthracene
Concen: 4.661 ng
RT: 17.163 min Scan# 1415
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:178 Resp: 1268387
Ion Ratio Lower Upper
178 100
176 18.2 14.6 22.0
179 15.5 12.2 18.4


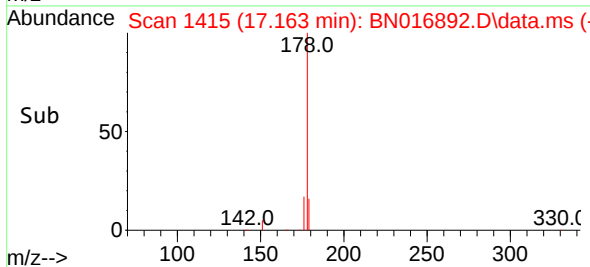

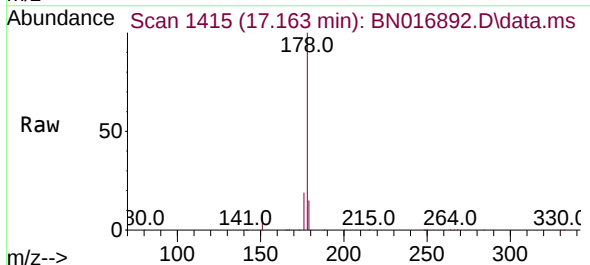


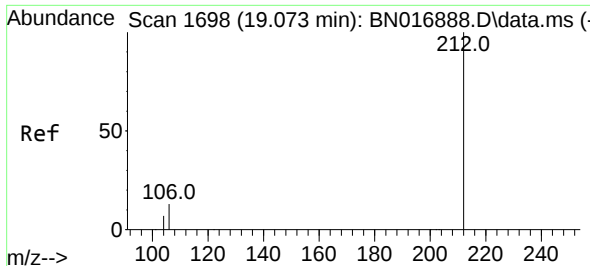

#27
Fluoranthene-d10
Concen: 4.461 ng
RT: 19.073 min Scan# 1698
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:212 Resp: 1277858
Ion Ratio Lower Upper
212 100
106 13.7 10.8 16.2
104 7.5 5.9 8.9

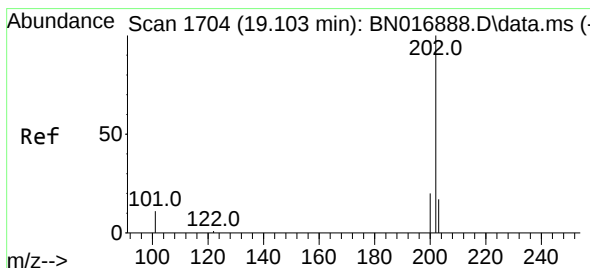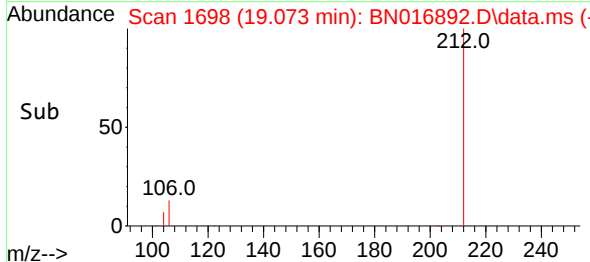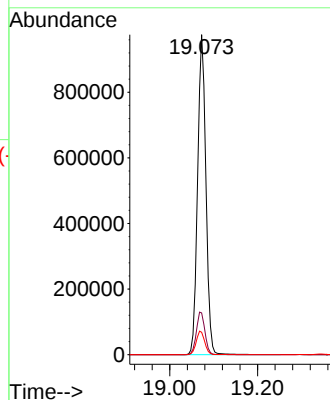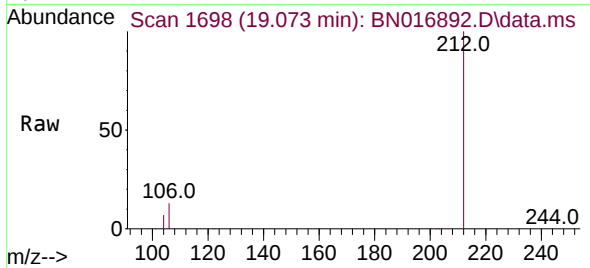

#28
Fluoranthene
Concen: 4.219 ng
RT: 19.103 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:202 Resp: 1451044
Ion Ratio Lower Upper
202 100
101 11.6 9.0 13.6
203 17.7 13.8 20.8


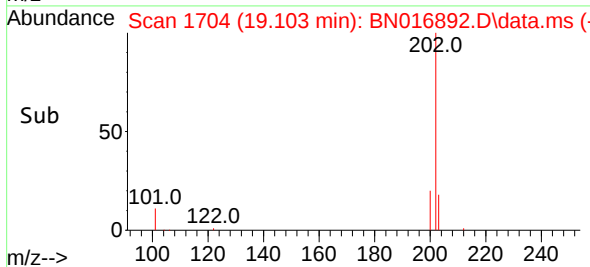
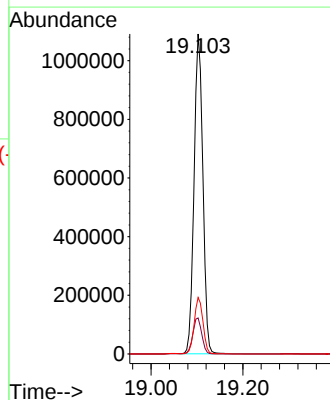
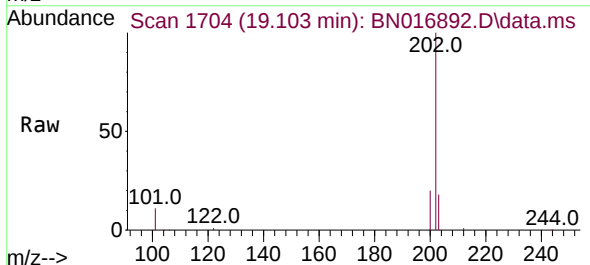




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.227 min Scan# 2001
Delta R.T. -0.011 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:240 Resp: 98570
Ion Ratio Lower Upper
240 100
120 14.5 4.1 6.1#
236 26.7 20.1 30.1

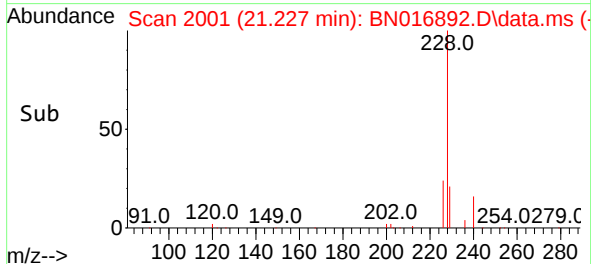

#30
Pyrene
Concen: 5.049 ng
RT: 19.465 min Scan# 1777
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:202 Resp: 1530286
Ion Ratio Lower Upper
202 100
200 20.6 16.4 24.6
203 17.8 14.0 21.0


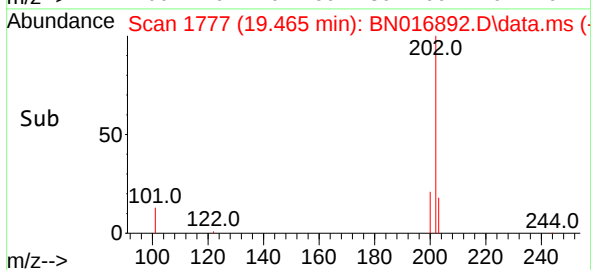

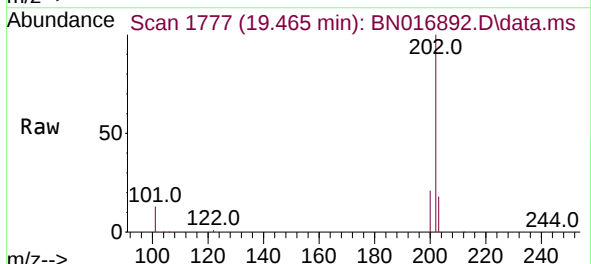




#31
 Terphenyl-d14
 Concen: 4.962 ng
 RT: 19.683 min Scan# 1821
 Delta R.T. -0.000 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0


Tgt Ion:244 Resp: 1066579
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.5 8.3
 122 11.0 8.6 13.0

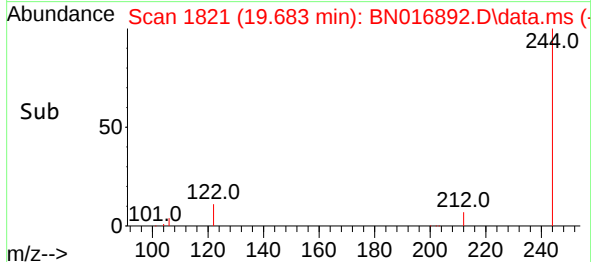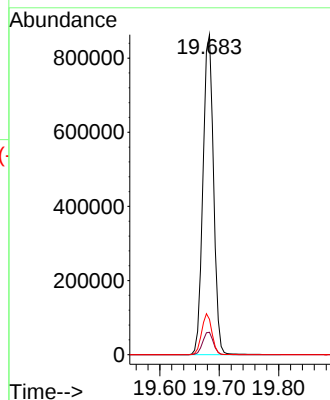

#32
 Benzo(a)anthracene
 Concen: 5.008 ng
 RT: 21.217 min Scan# 2000
 Delta R.T. -0.000 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Tgt Ion:228 Resp: 1526709
 Ion Ratio Lower Upper
 228 100
 226 26.3 21.2 31.8
 229 20.2 15.8 23.6



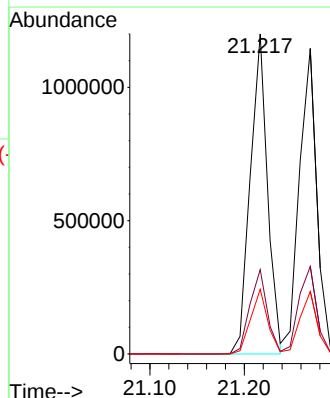
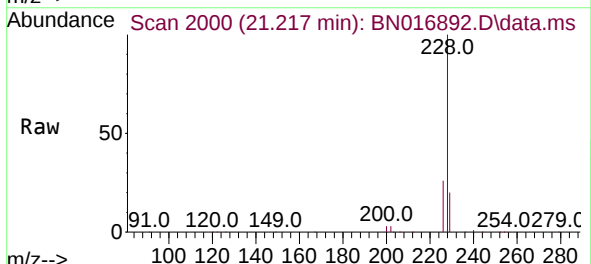


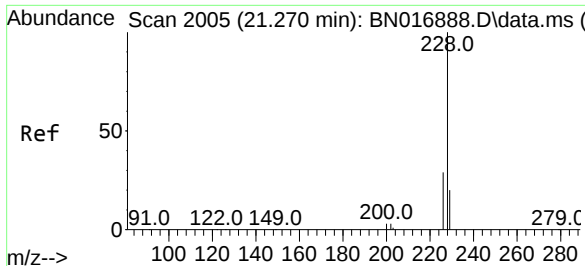

#33
Chrysene
Concen: 4.739 ng
RT: 21.270 min Scan# 2005
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:228 Resp: 1471399
Ion Ratio Lower Upper
228 100
226 28.7 23.3 34.9
229 20.5 15.8 23.6

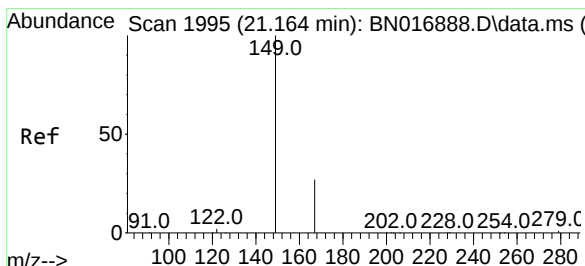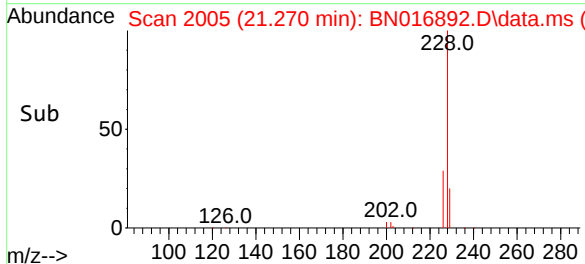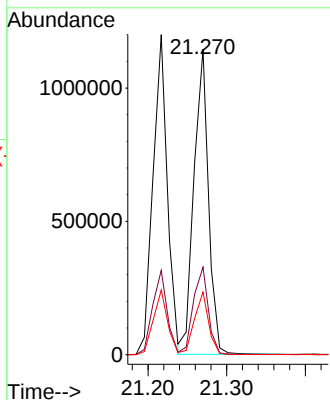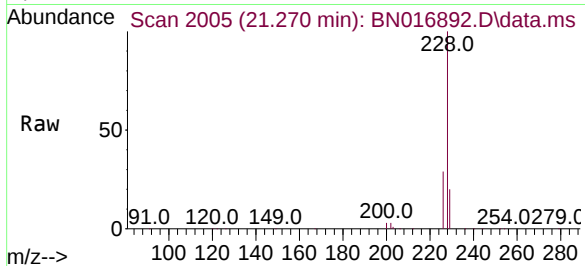

#34
Bis(2-ethylhexyl)phthalate
Concen: 6.611 ng
RT: 21.164 min Scan# 1995
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:149 Resp: 1024101
Ion Ratio Lower Upper
149 100
167 28.5 22.2 33.2
279 4.6 3.5 5.3

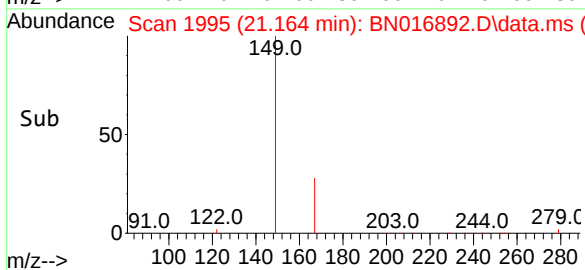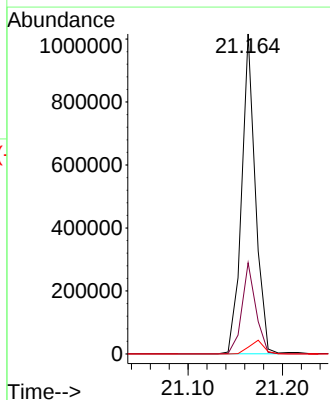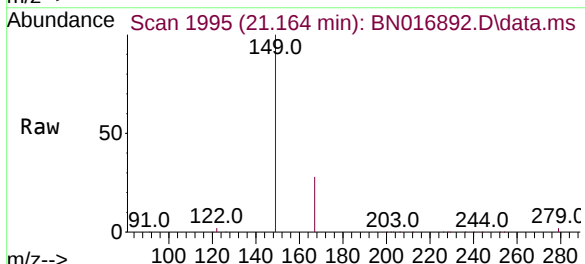







#35
Perylene-d12
Concen: 0.400 ng
RT: 23.478 min Scan# 2425
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0

Tgt Ion:264 Resp: 106176




Ion	Ratio	Lower	Upper
264	100		
260	24.2	19.4	29.2
265	23.6	19.2	28.8

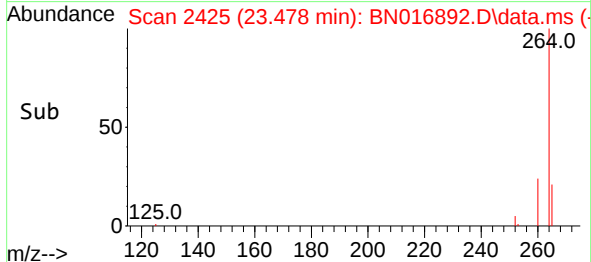


#36
Indeno(1,2,3-cd)pyrene
Concen: 4.654 ng
RT: 25.750 min Scan# 3089
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:276 Resp: 1871447

Ion	Ratio	Lower	Upper
276	100		
138	24.5	20.1	30.1
277	25.2	20.1	30.1




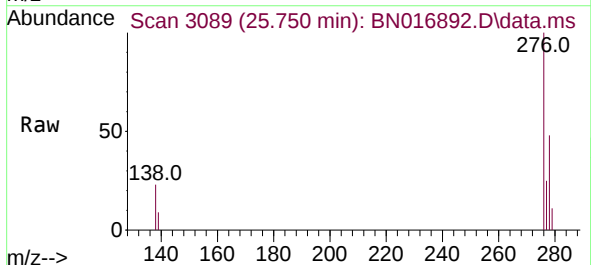




#37
Benzo(b)fluoranthene
Concen: 4.812 ng
RT: 22.800 min Scan# 21
Delta R.T. -0.003 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34




Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0


Tgt Ion:252 Resp: 1617155
Ion Ratio Lower Upper
252 100
253 22.1 17.8 26.8
125 9.9 8.1 12.1

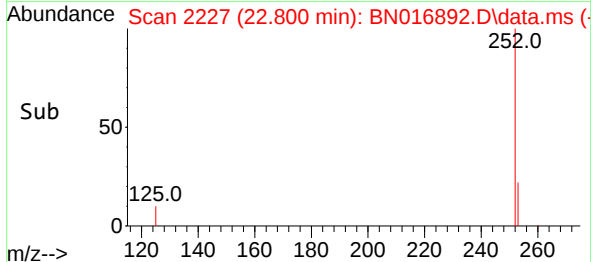

#38
Benzo(k)fluoranthene
Concen: 4.772 ng
RT: 22.848 min Scan# 2241
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34


Tgt Ion:252 Resp: 1559175
Ion Ratio Lower Upper
252 100
253 22.2 18.0 27.0
125 9.9 9.0 13.6

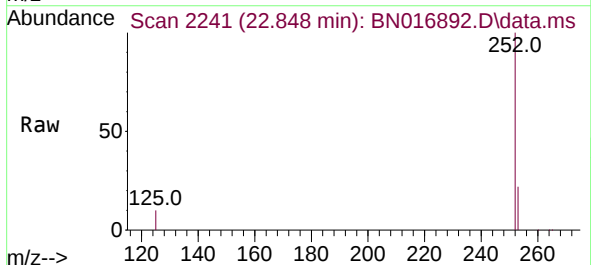






#39
Benzo(a)pyrene
Concen: 4.892 ng
RT: 23.378 min Scan# 2396
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Instrument :
BNA_N
ClientSampleId :
SSTDICC5.0







Tgt Ion:252 Resp: 1502200
Ion Ratio Lower Upper
252 100
253 22.0 17.8 26.8
125 10.8 9.0 13.6

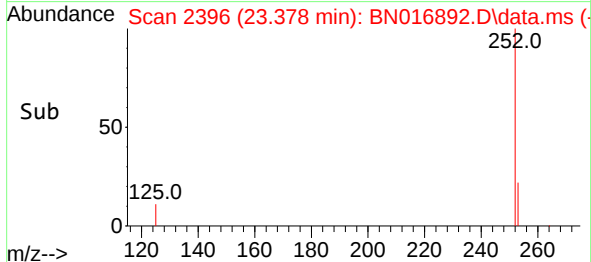

#40
Dibenzo(a,h)anthracene
Concen: 4.703 ng
RT: 25.771 min Scan# 3095
Delta R.T. -0.000 min
Lab File: BN016892.D
Acq: 11 Oct 2021 21:34

Tgt Ion:278 Resp: 1547921
Ion Ratio Lower Upper
278 100
139 16.0 13.4 20.0
279 23.8 19.2 28.8

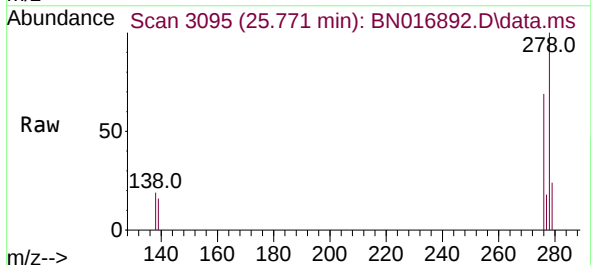

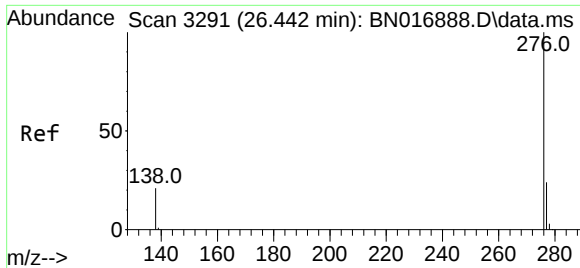

#41
 Benzo(g,h,i)perylene
 Concen: 4.637 ng
 RT: 26.445 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: BN016892.D
 Acq: 11 Oct 2021 21:34

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC5.0

Tgt Ion:276 Resp: 1621354
 Ion Ratio Lower Upper
 276 100
 277 23.9 19.0 28.6
 138 20.9 16.7 25.1

