
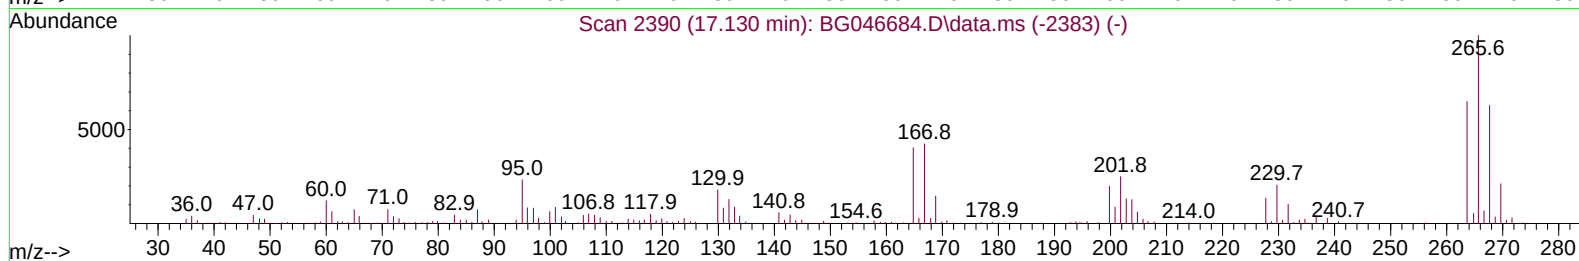
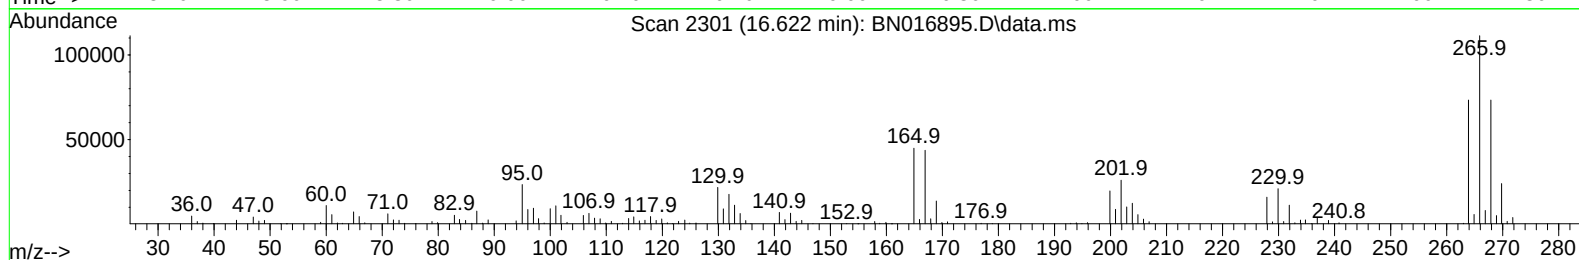


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016895.D
Acq On : 12 Oct 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:27:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 18:26:37 2021
Response via : Initial Calibration

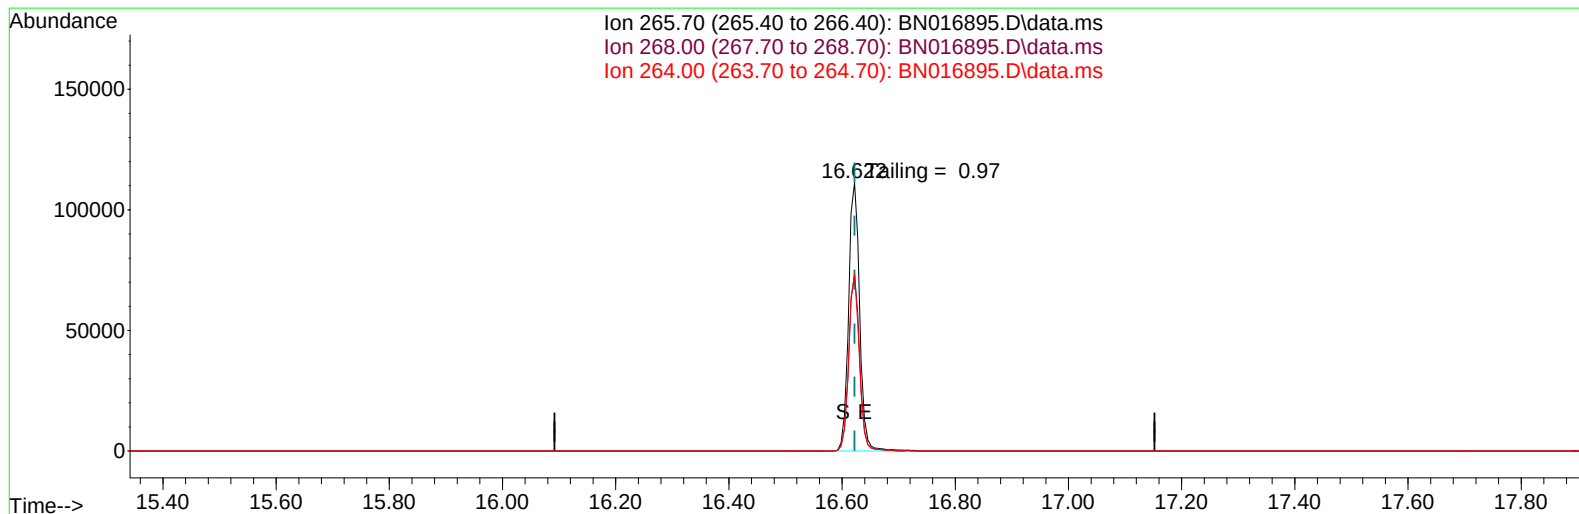

TIC: BN016895.D\data.ms

(70) Pentachlorophenol (C)




16.622min (0.000) 31874.84 ng

response 151088

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.87
264.00	61.60	65.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016895.D
Acq On : 12 Oct 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 18:27:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 18:26:37 2021
Response via : Initial Calibration

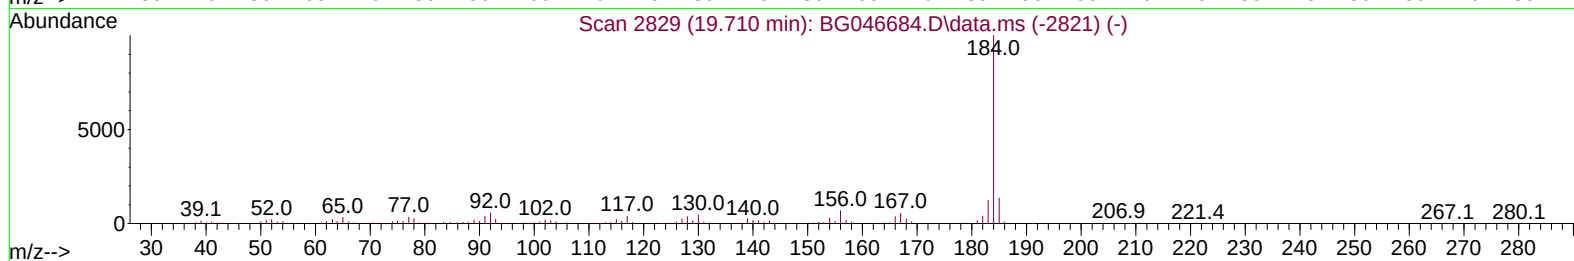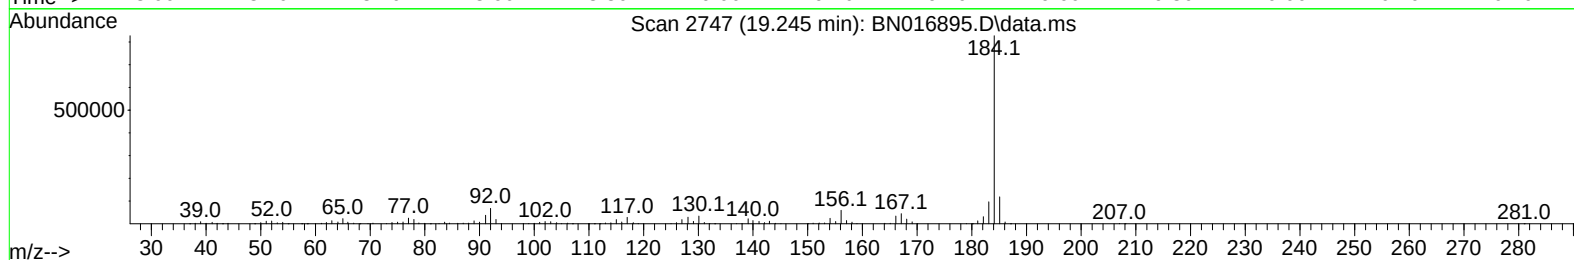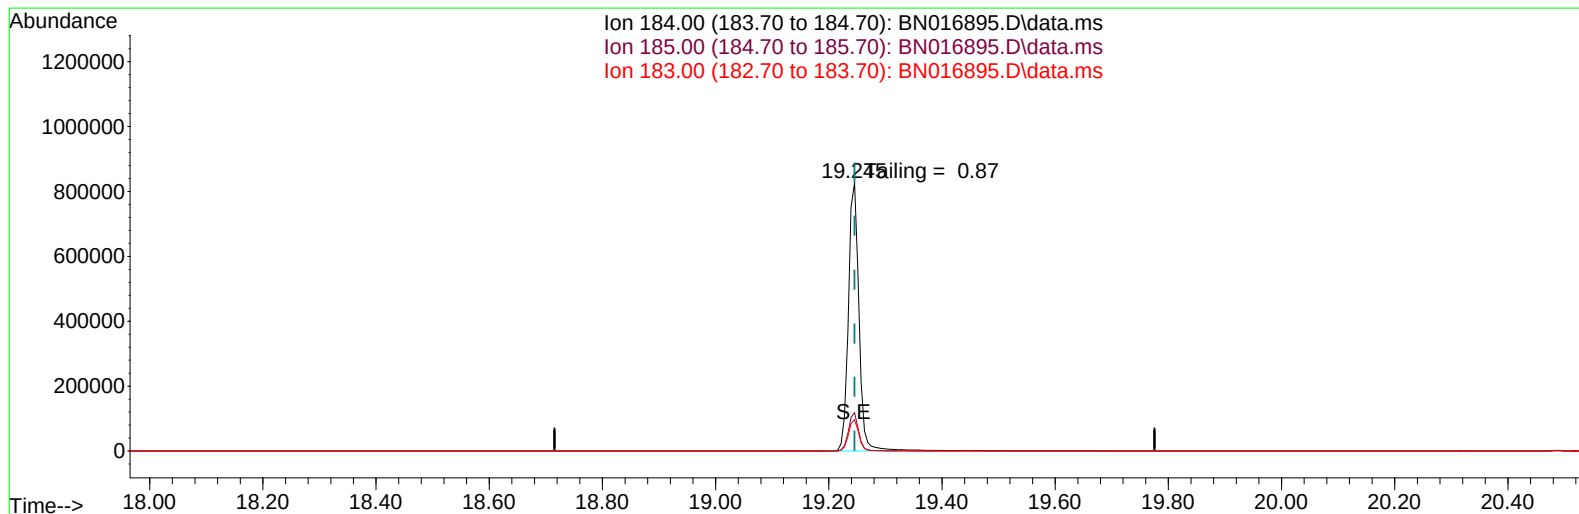

TIC: BN016895.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 1073748

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.69
0.00	0.00	0.00