


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
 Data File : BN016885.D
 Acq On : 11 Oct 2021 16:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 12 02:31:22 2021

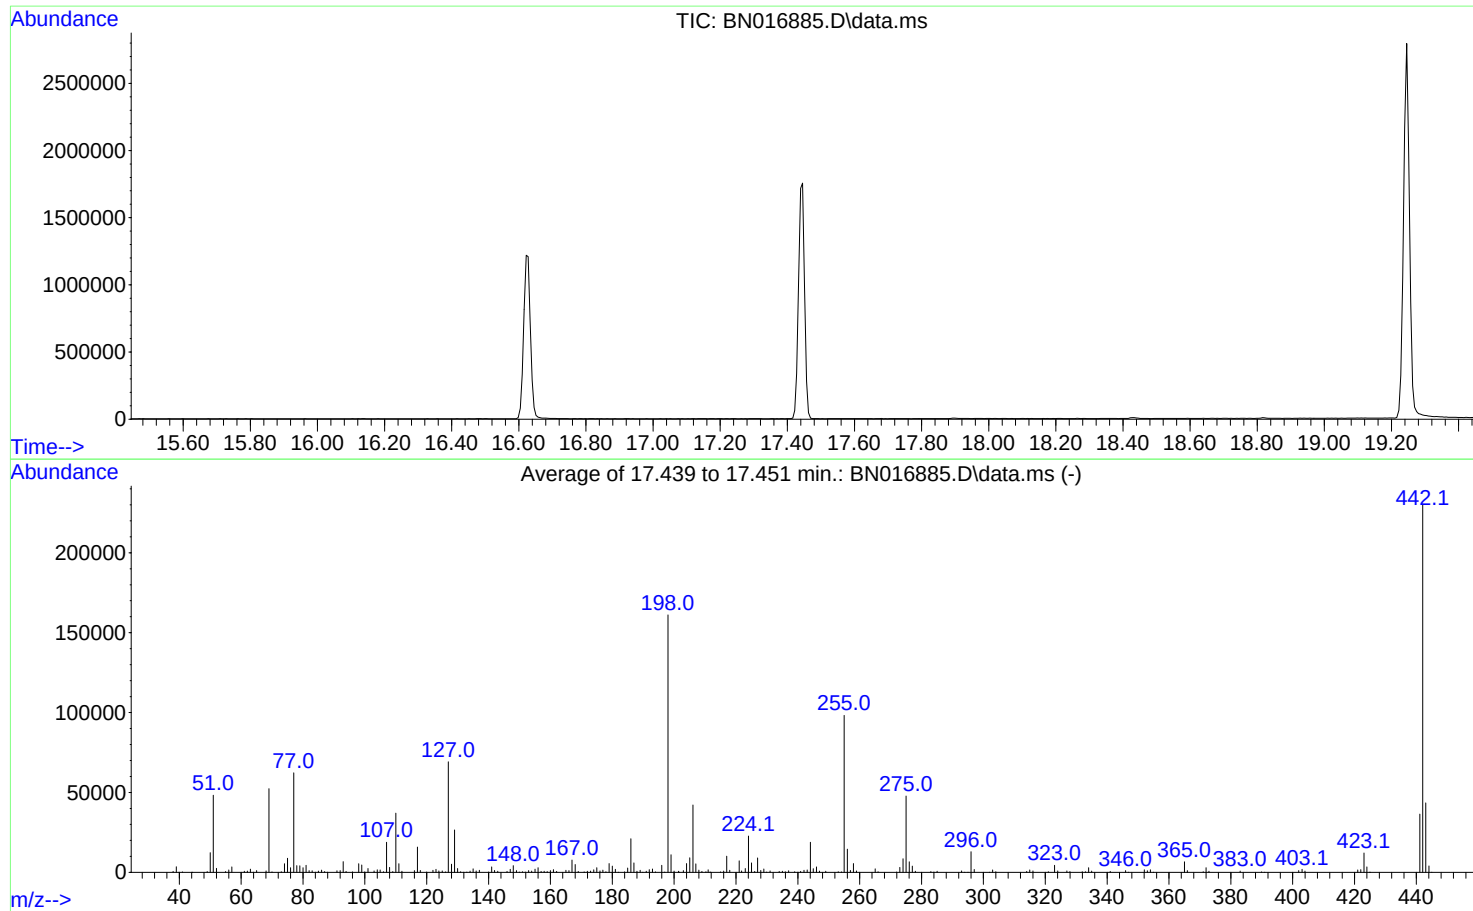




AutoFind: Scans 2440, 2441, 2442; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	48288	PASS
68	69	0.00	2	1.7	910	PASS
69	198	0.00	100	32.5	52411	PASS
70	69	0.00	2	0.5	274	PASS
127	198	10	80	42.9	69187	PASS
197	198	0.00	2	0.1	209	PASS
198	198	100	100	100.0	161131	PASS
199	198	5	9	6.8	11019	PASS
275	198	10	60	29.6	47741	PASS
365	198	1	100	4.1	6584	PASS
441	198	0.01	100	22.6	36496	PASS
442	442	50	100	100.0	230229	PASS
443	442	15	24	18.9	43440	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016885.D
Acq On : 11 Oct 2021 16:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 02:55:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 02:55:50 2021
Response via : Initial Calibration

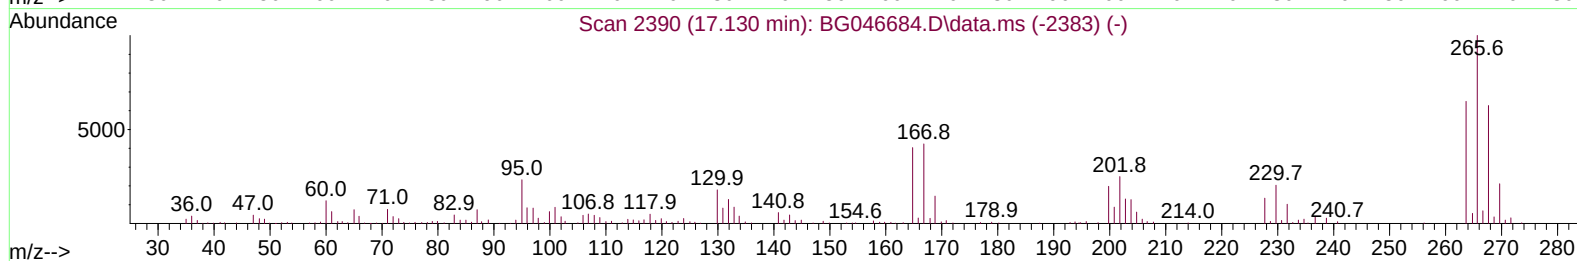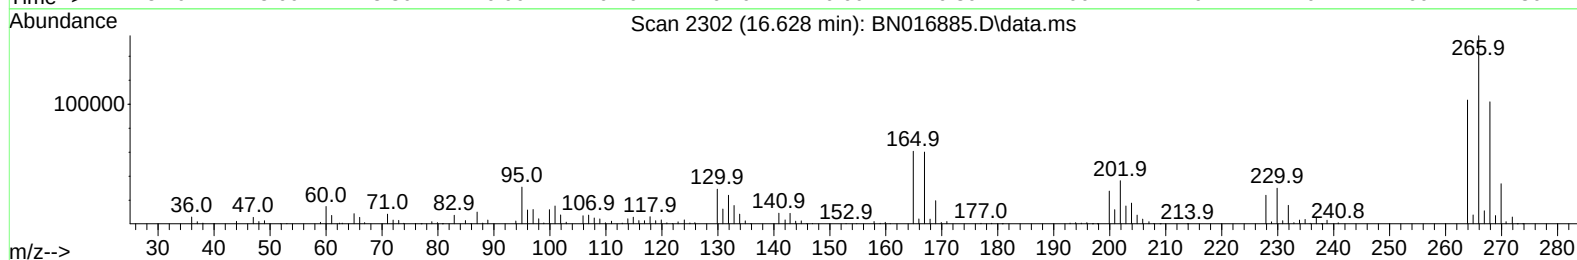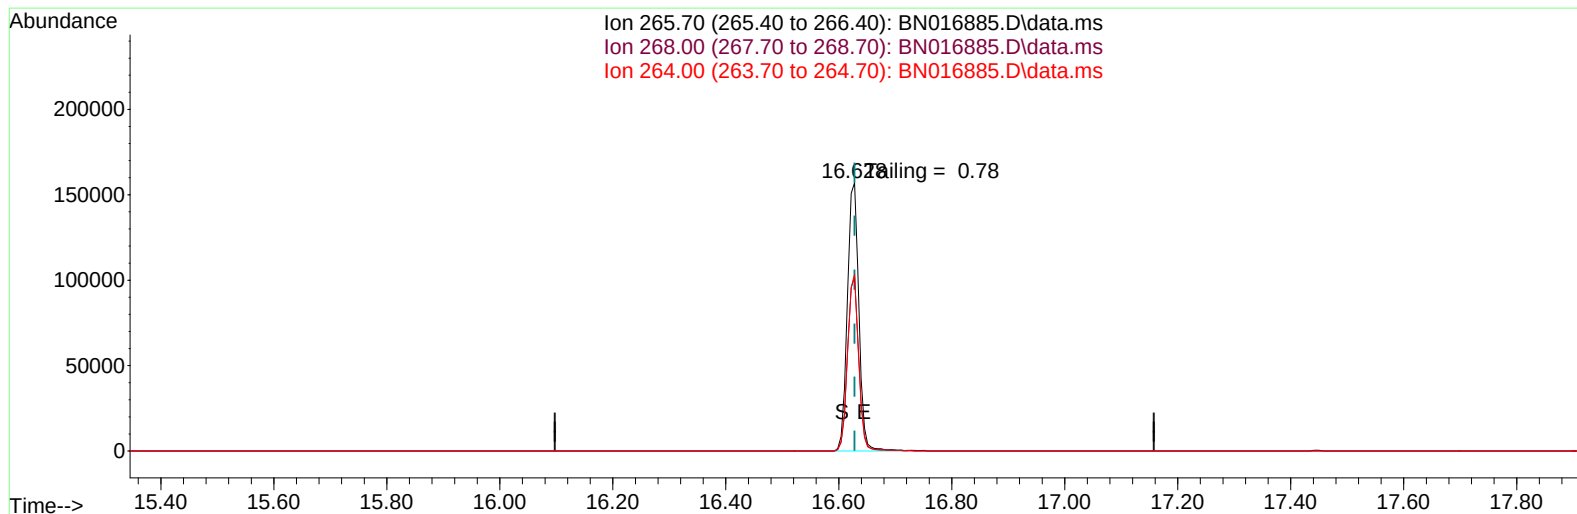

TIC: BN016885.D\data.ms

(70) Pentachlorophenol (C)

16.628min (0.000) 30731.95 ng




response 222606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.95
264.00	61.60	65.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016885.D
Acq On : 11 Oct 2021 16:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 02:55:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 02:55:50 2021
Response via : Initial Calibration

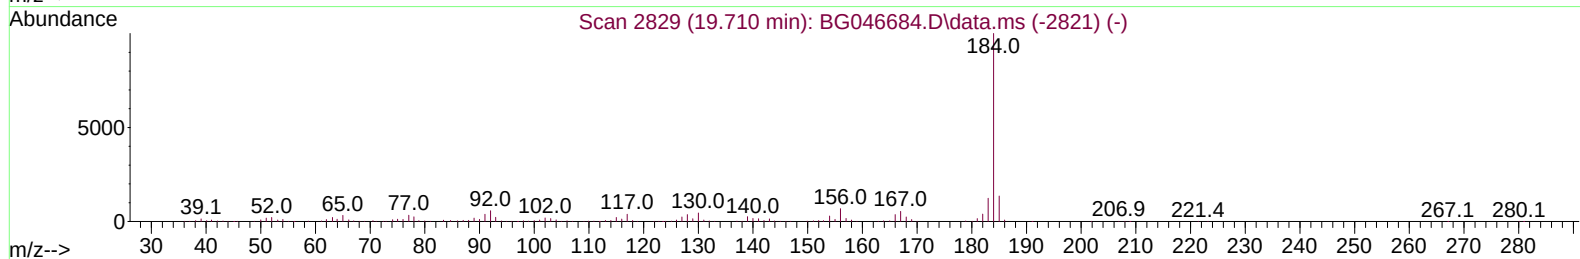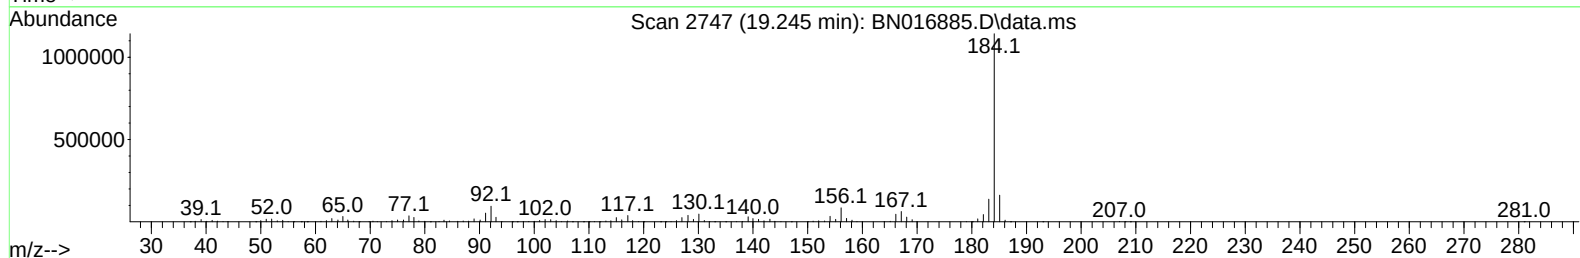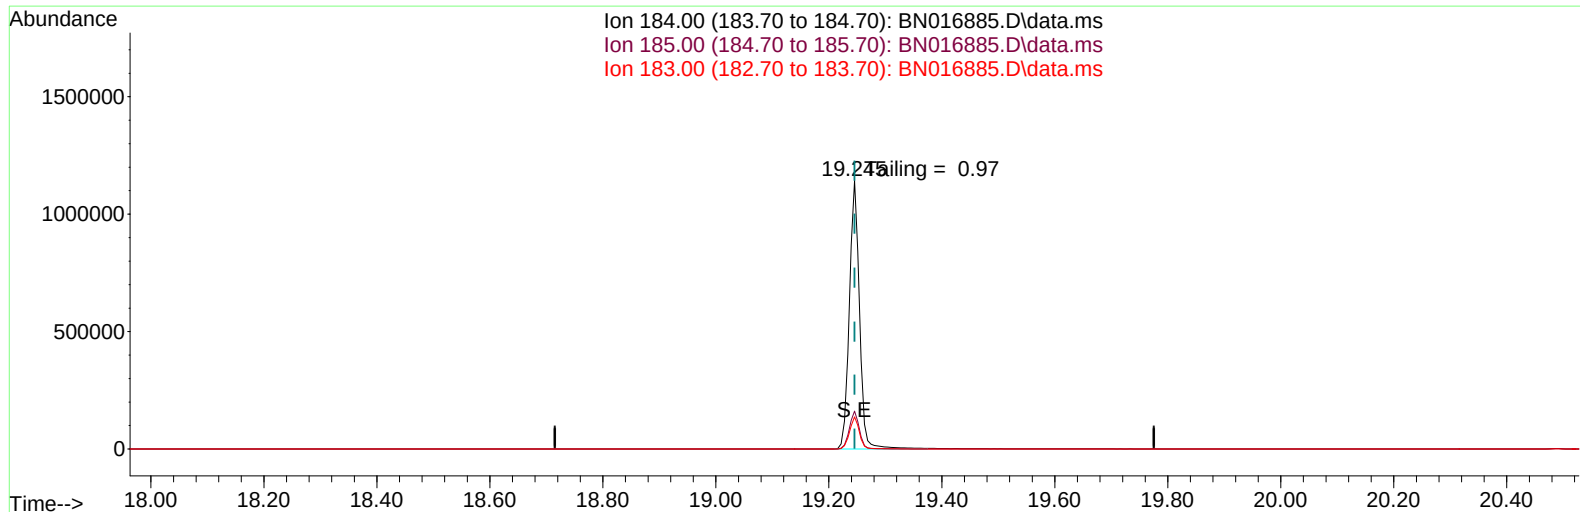

TIC: BN016885.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 1439827

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.17
183.00	13.20	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2021	BNA_N	<u>BN016885.D</u>
Compound Name	Response	Retention Time
DDT	671839	20.486
DDD	2836	20.098
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2836	674675	0.42

Instrument :
BNA_N
ClientSampleId :
DFTPP