


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
 Data File : BN016895.D
 Acq On : 12 Oct 2021 08:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN101221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Oct 12 02:31:22 2021

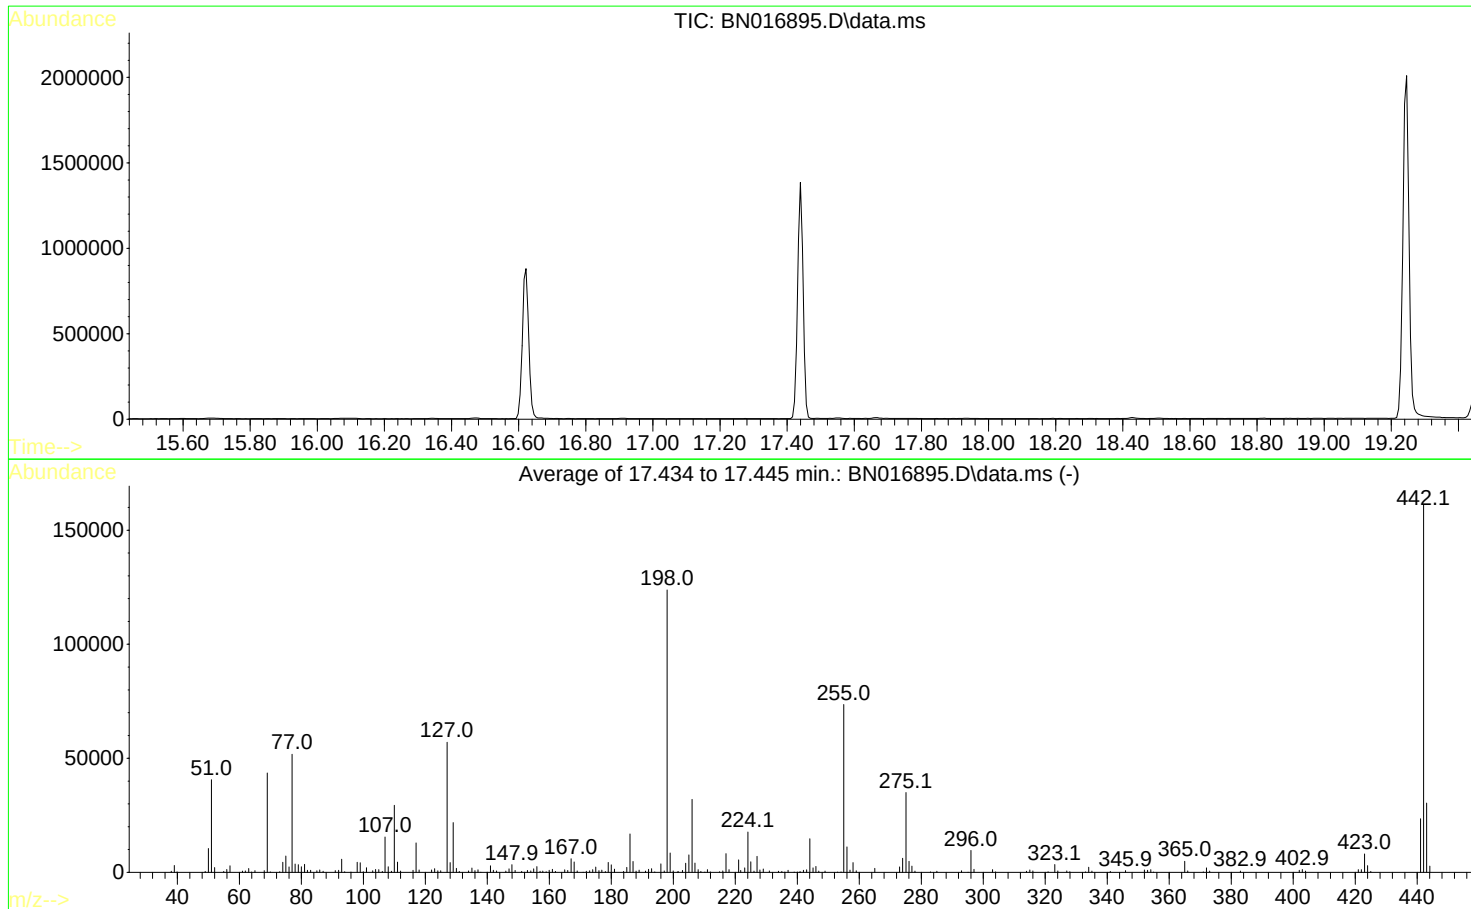




AutoFind: Scans 2439, 2440, 2441; Background Corrected with Scan 2433

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	40611	PASS
68	69	0.00	2	1.9	811	PASS
69	198	0.00	100	35.2	43565	PASS
70	69	0.00	2	0.5	225	PASS
127	198	10	80	46.1	57061	PASS
197	198	0.00	2	0.5	630	PASS
198	198	100	100	100.0	123811	PASS
199	198	5	9	6.9	8484	PASS
275	198	10	60	28.3	35013	PASS
365	198	1	100	3.9	4867	PASS
441	198	0.01	100	19.0	23509	PASS
442	442	50	100	100.0	161275	PASS
443	442	15	24	18.8	30365	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016895.D
Acq On : 12 Oct 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 18:27:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 18:26:37 2021
Response via : Initial Calibration

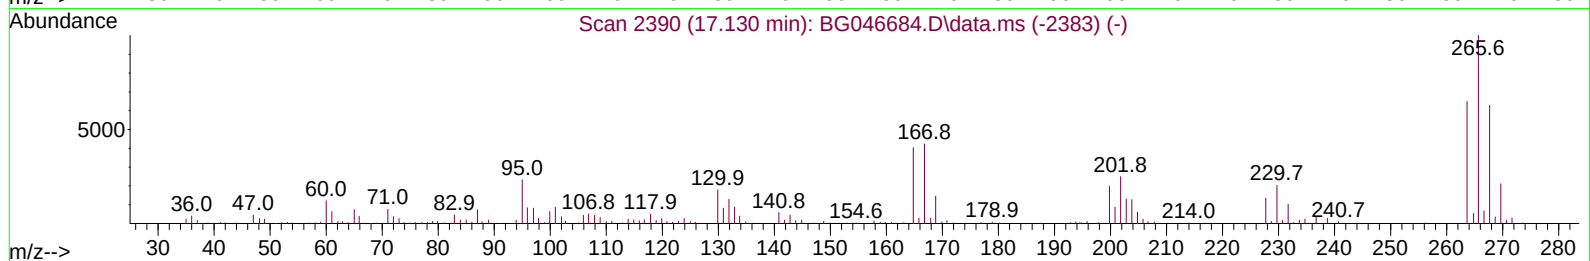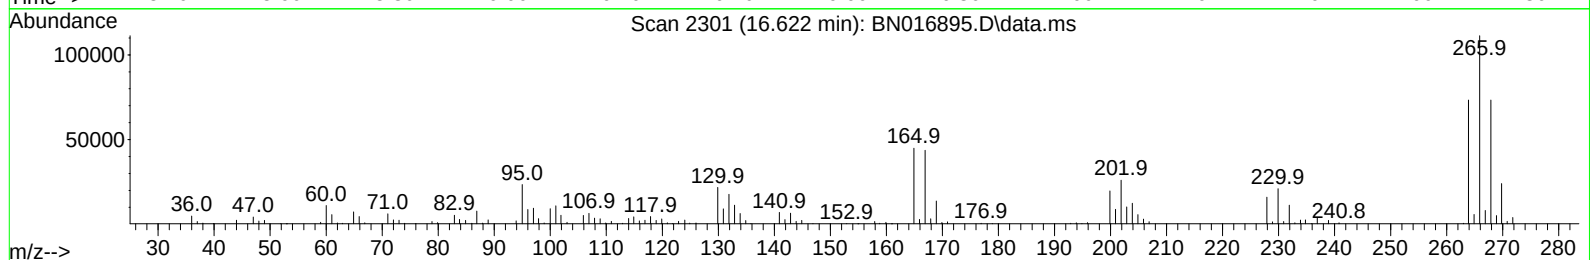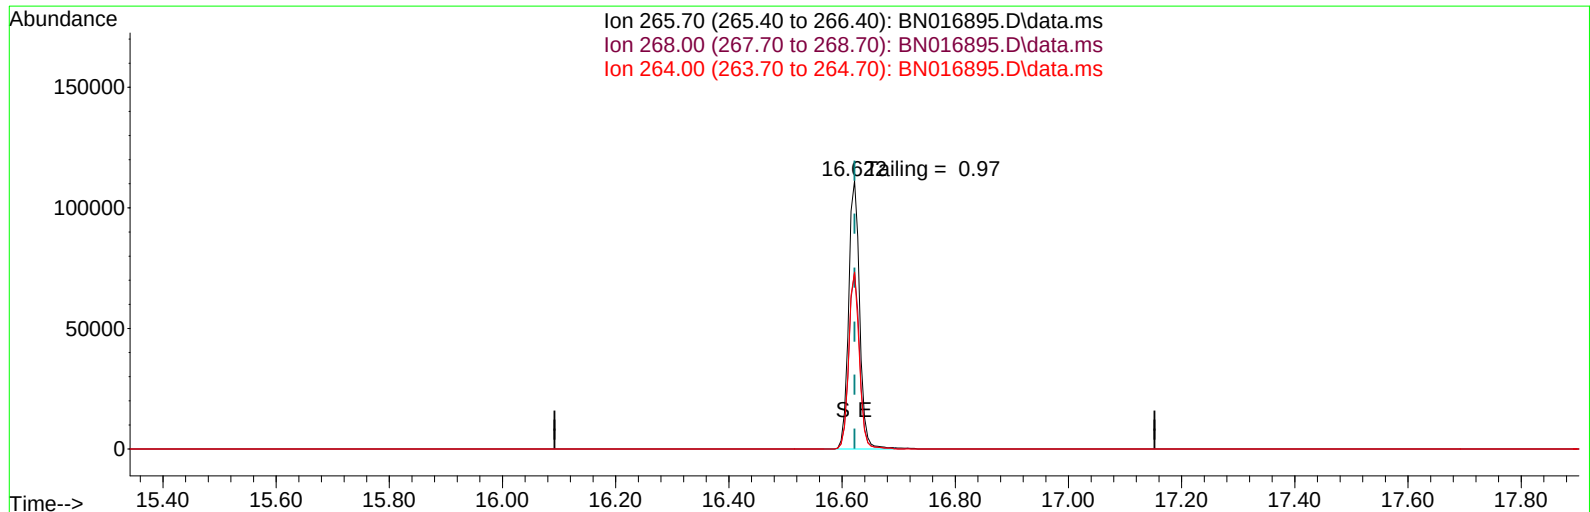

TIC: BN016895.D\data.ms

(70) Pentachlorophenol (C)

16.622min (0.000) 31874.84 ng




response 151088

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.87
264.00	61.60	65.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101221\
Data File : BN016895.D
Acq On : 12 Oct 2021 08:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 12 18:27:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 12 18:26:37 2021
Response via : Initial Calibration

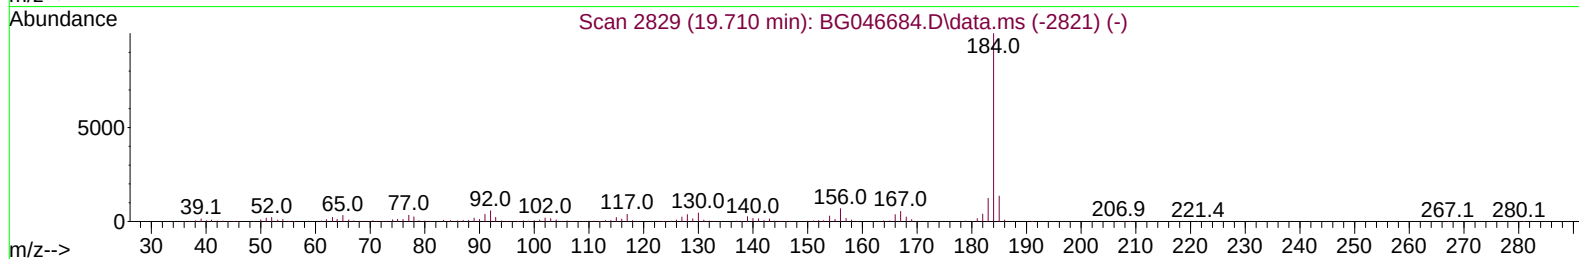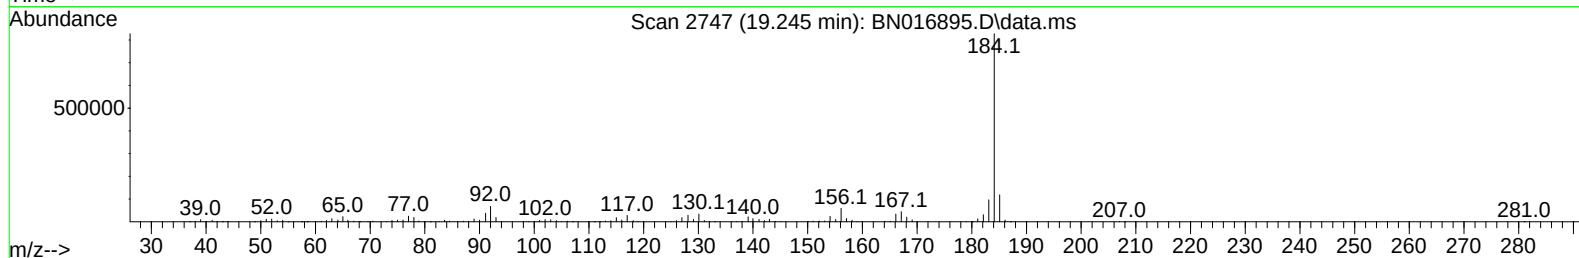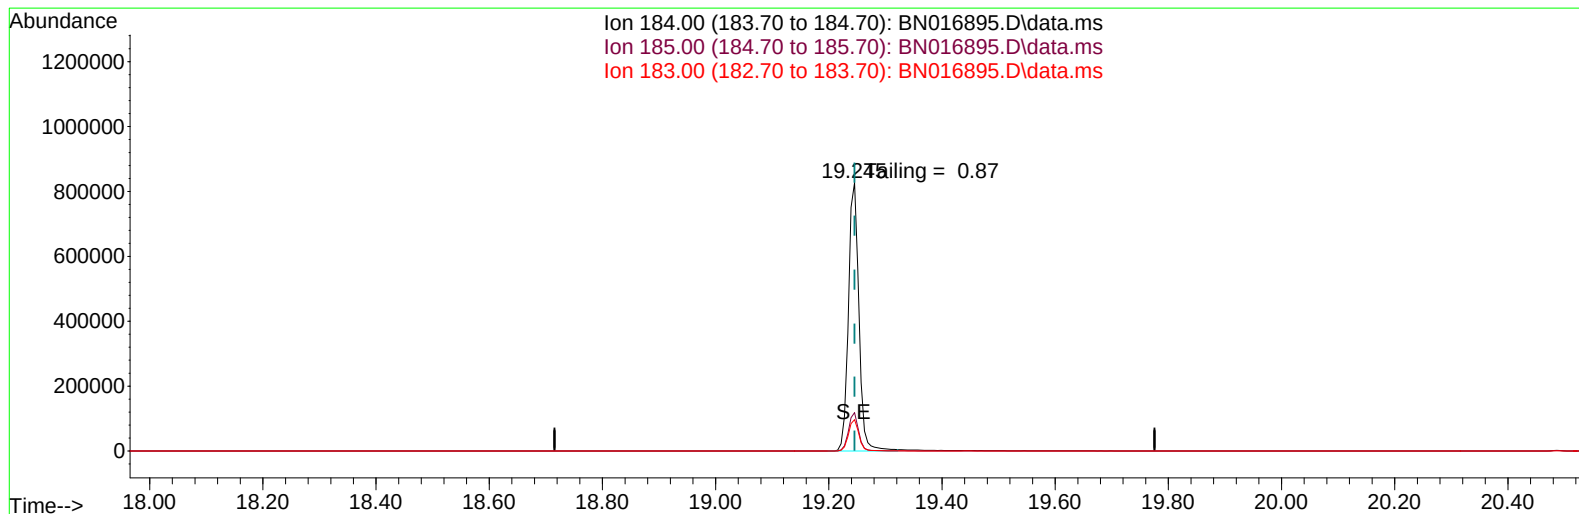

TIC: BN016895.D\data.ms

(77) Benzidine

19.245min (0.000) 0.00 ng

response 1073748

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.29
183.00	13.20	11.69
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/12/2021	BNA_N	<u>BN016895.D</u>
Compound Name	Response	Retention Time
DDT	500920	20.486
DDD	623	20.05
DDE	0	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
623	501543	0.12

Instrument :
BNA_N
ClientSampleId :
DFTPP