
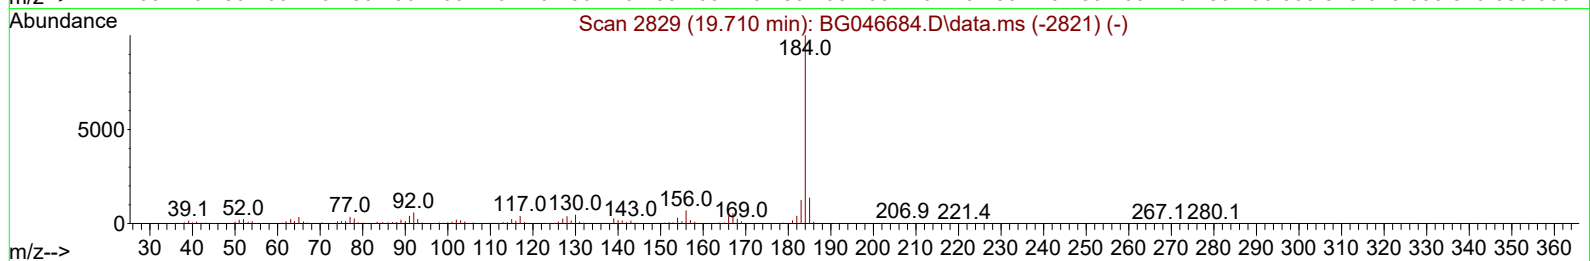
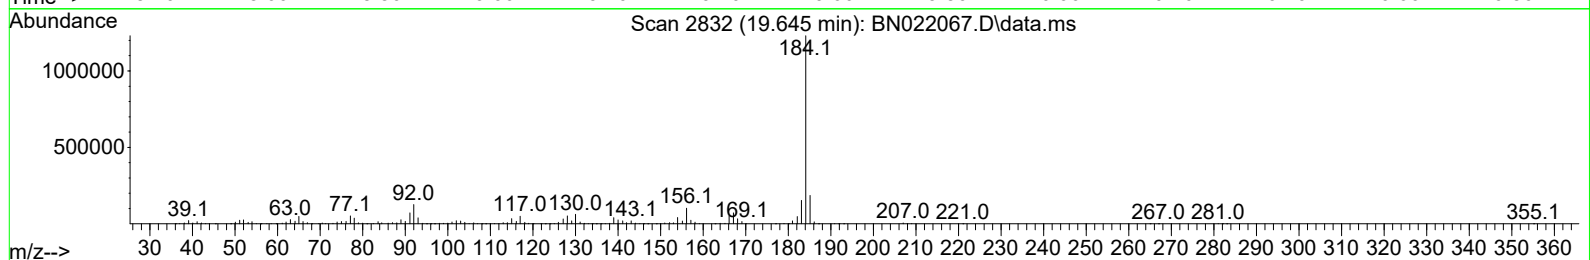


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101322\
Data File : BN022067.D
Acq On : 12 Oct 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 09:30:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 09:30:43 2022
Response via : Initial Calibration

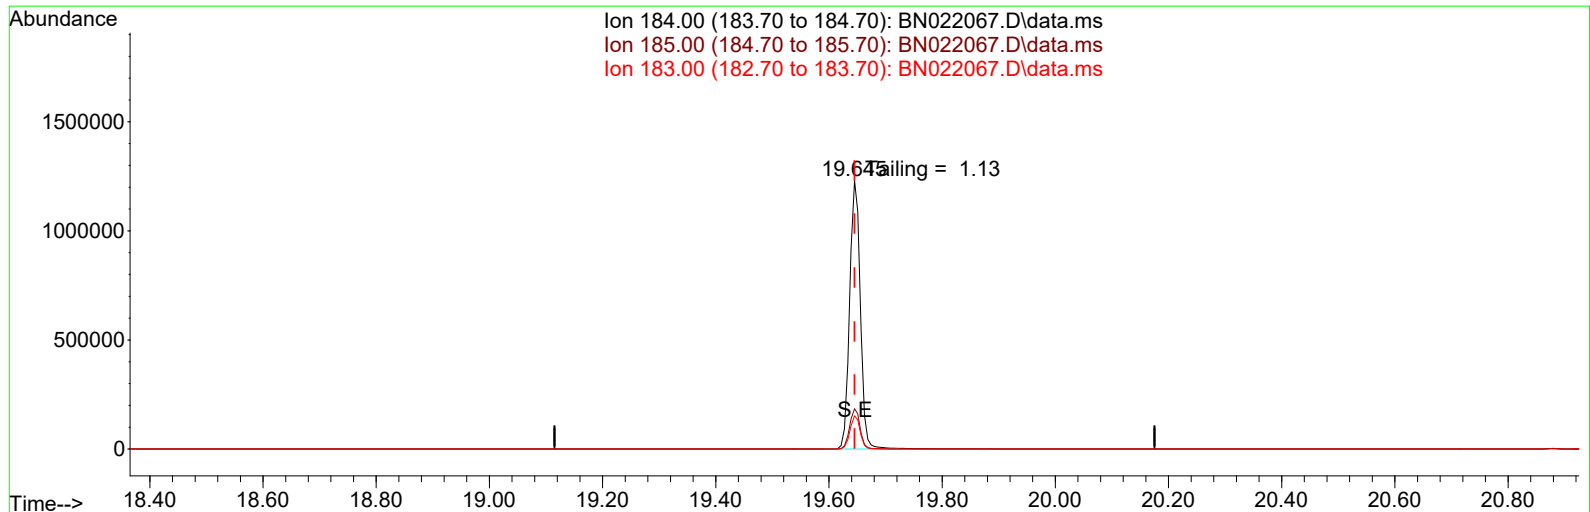

TIC: BN022067.D\data.ms

(77) Benzidine




19.645min (0.000) 385488.37 ng

response 1604181

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	12.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101322\
Data File : BN022067.D
Acq On : 12 Oct 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 13 09:30:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 09:30:43 2022
Response via : Initial Calibration

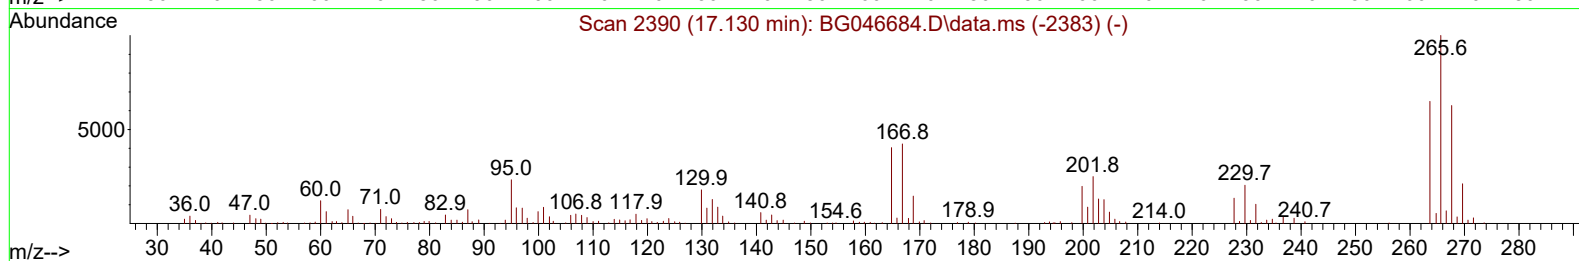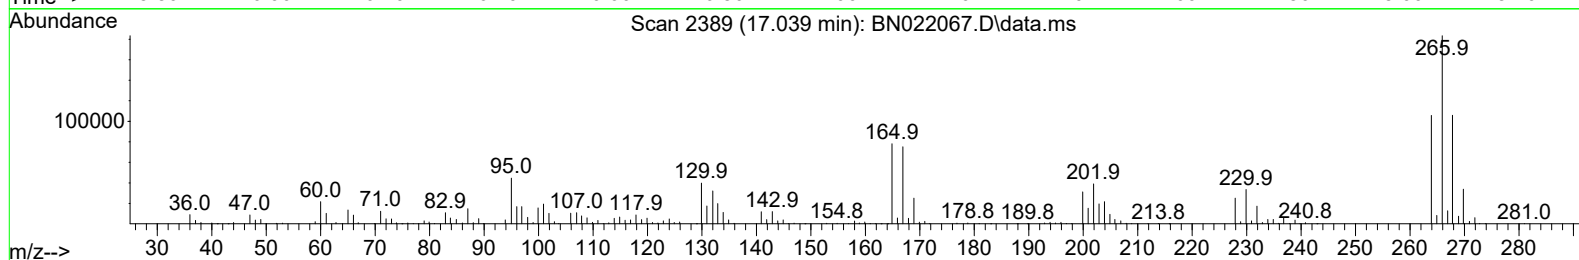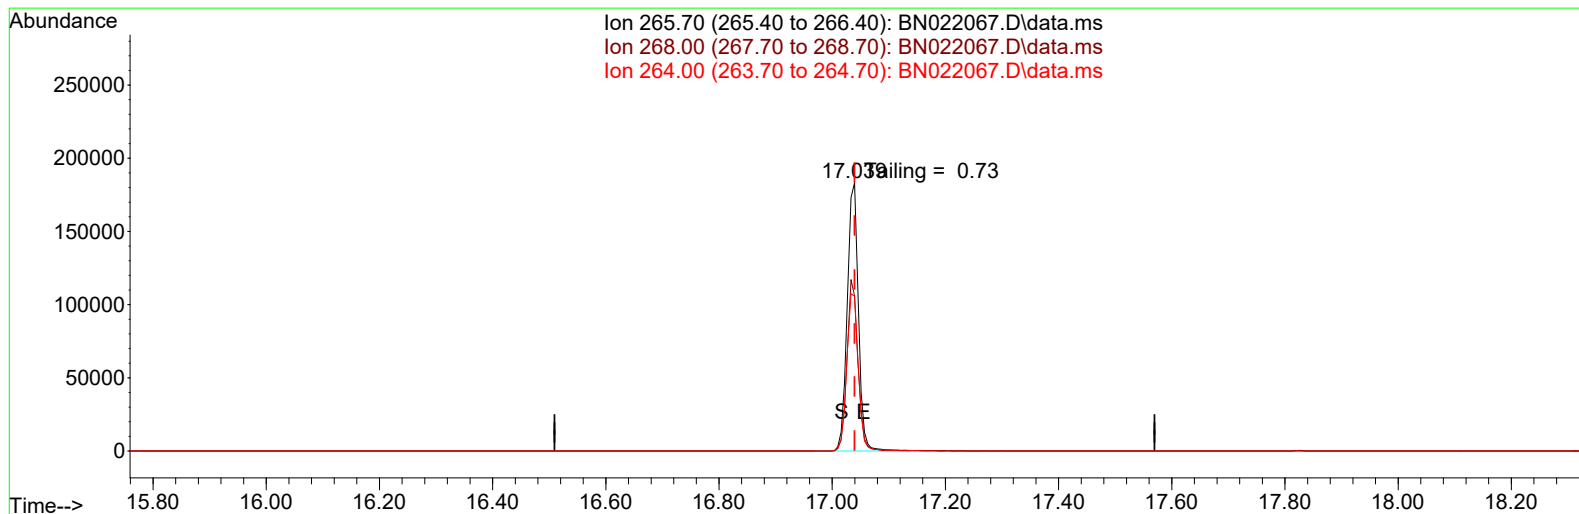

TIC: BN022067.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 22076.46 ng m

response 251040

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	57.68
0.00	0.00	0.00