


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101322\
 Data File : BN022067.D
 Acq On : 12 Oct 2022 16:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 13 01:51:34 2022

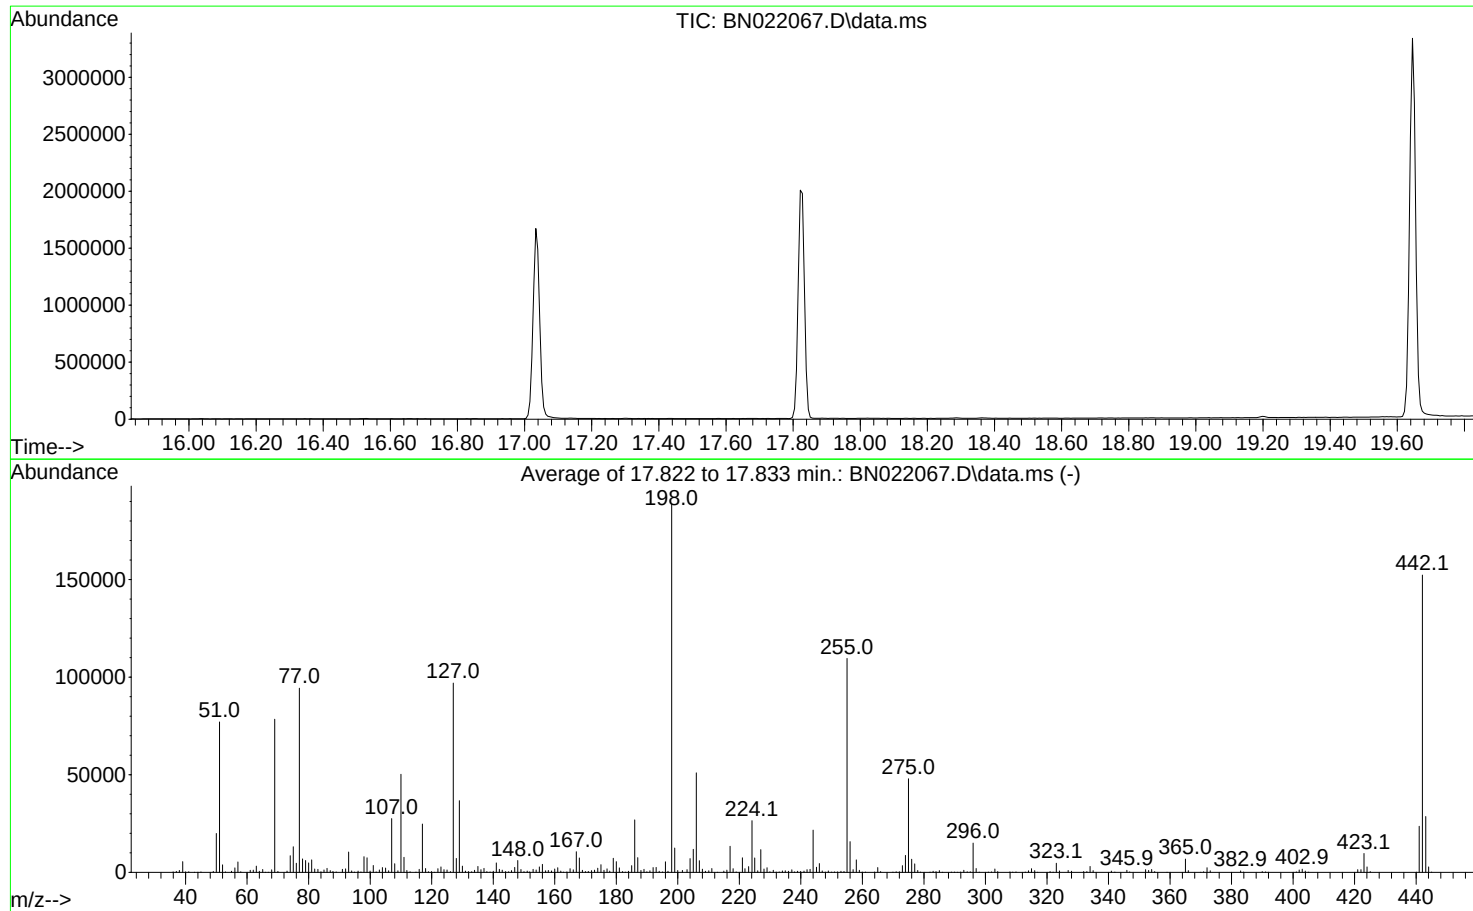




AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	77056	PASS
68	69	0.00	2	1.6	1292	PASS
69	198	0.00	100	41.6	78437	PASS
70	69	0.00	2	0.6	452	PASS
127	198	10	80	51.4	96976	PASS
197	198	0.00	2	0.3	522	PASS
198	198	100	100	100.0	188501	PASS
199	198	5	9	6.6	12452	PASS
275	198	10	60	25.4	47901	PASS
365	198	1	100	3.6	6728	PASS
441	198	0.01	100	12.5	23549	PASS
442	442	50	100	100.0	152341	PASS
443	442	15	24	18.8	28597	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101322\
 Data File : BN022067.D
 Acq On : 12 Oct 2022 16:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Oct 13 09:30:48 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 13 09:30:43 2022
 Response via : Initial Calibration

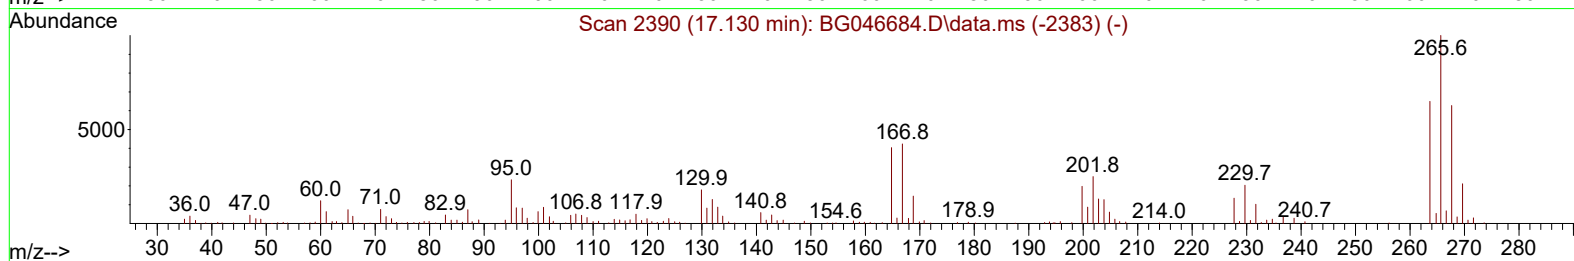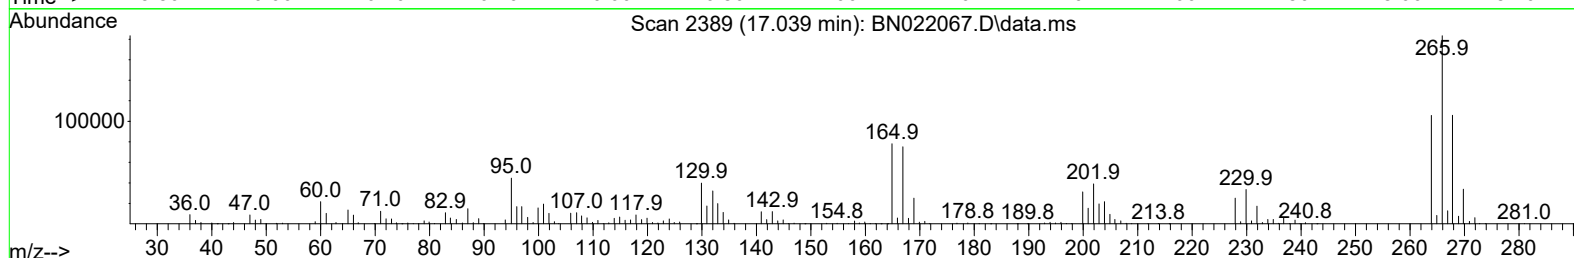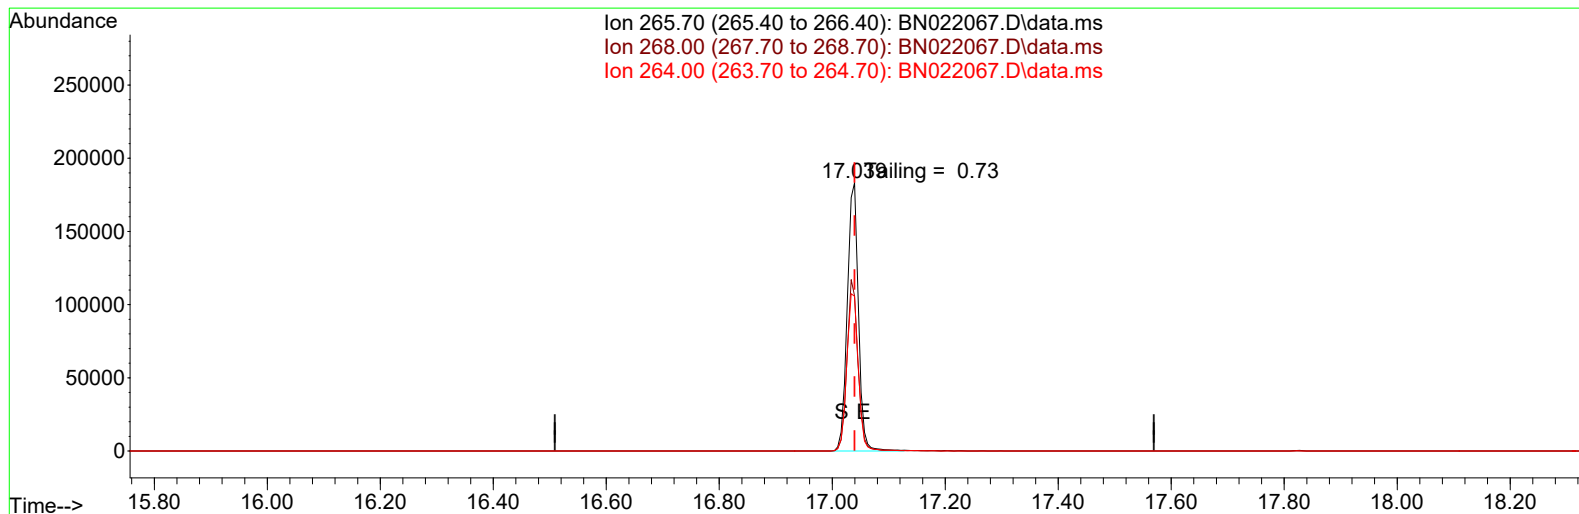

TIC: BN022067.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 22140.13 ng




response 251764

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	57.76
264.00	61.60	57.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN101322\
Data File : BN022067.D
Acq On : 12 Oct 2022 16:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Oct 13 09:30:48 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 13 09:30:43 2022
Response via : Initial Calibration

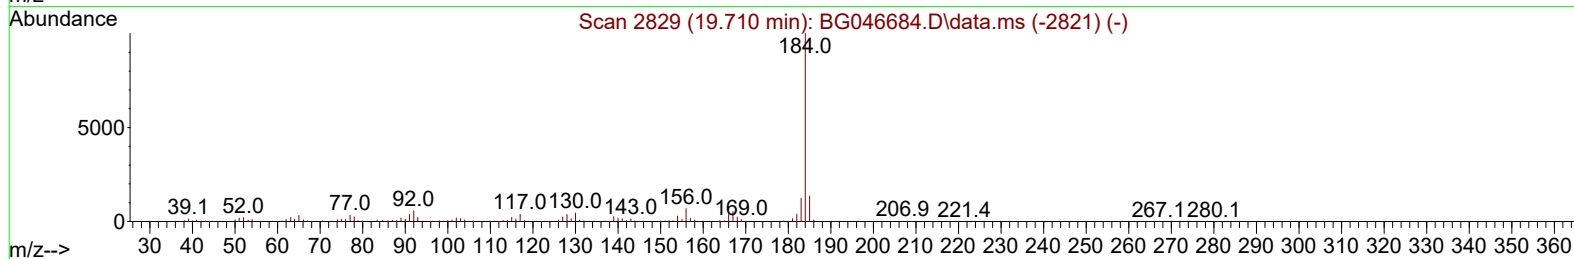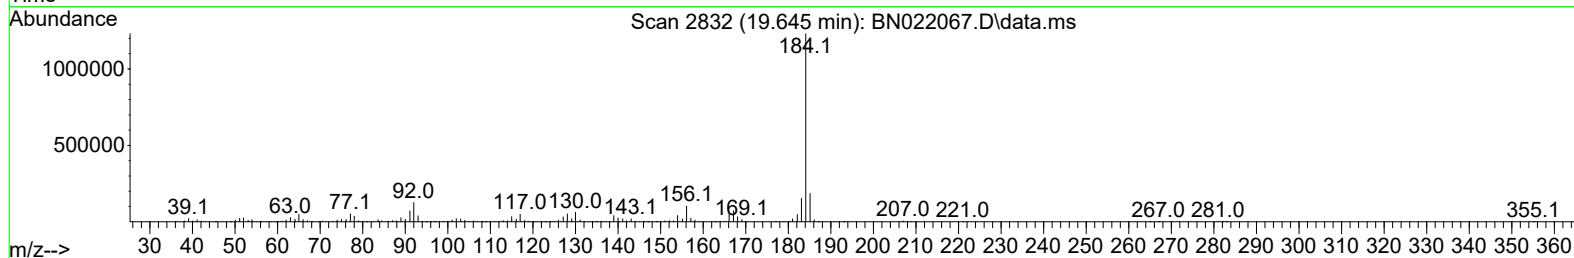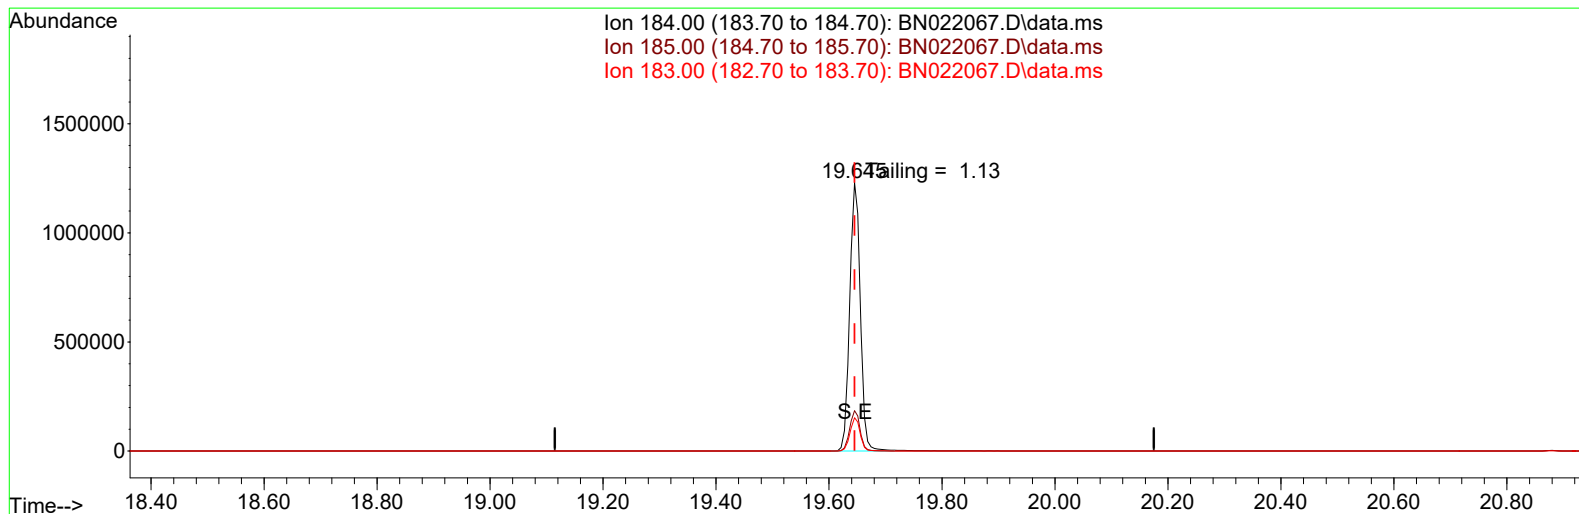

TIC: BN022067.D\data.ms

(77) Benzidine

19.645min (0.000) 385488.37 ng

response 1604181

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.04
183.00	13.20	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/13/2022	BNA_N	<u>BN022067.D</u>
Compound Name	Response	Retention Time
DDT	714985	20.88
DDD	6168	20.439
DDE	0	19.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6168	721153	0.86

Instrument :
BNA_N
ClientSampleId :
DFTPP