
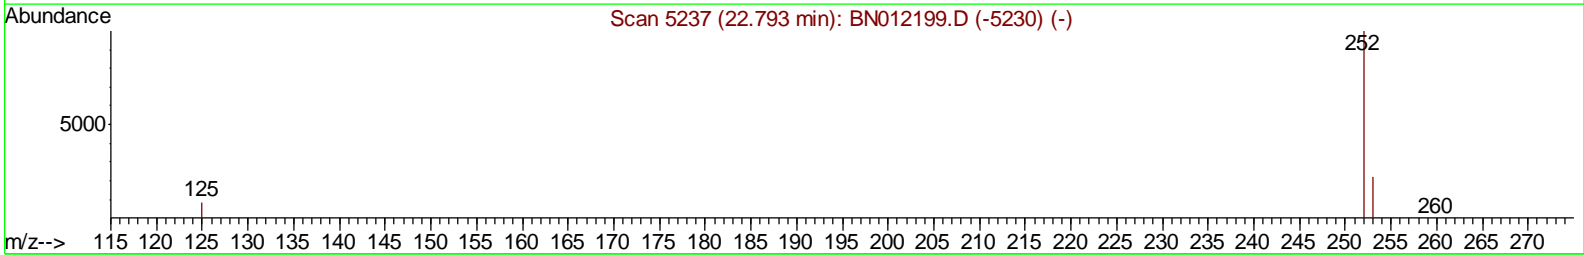
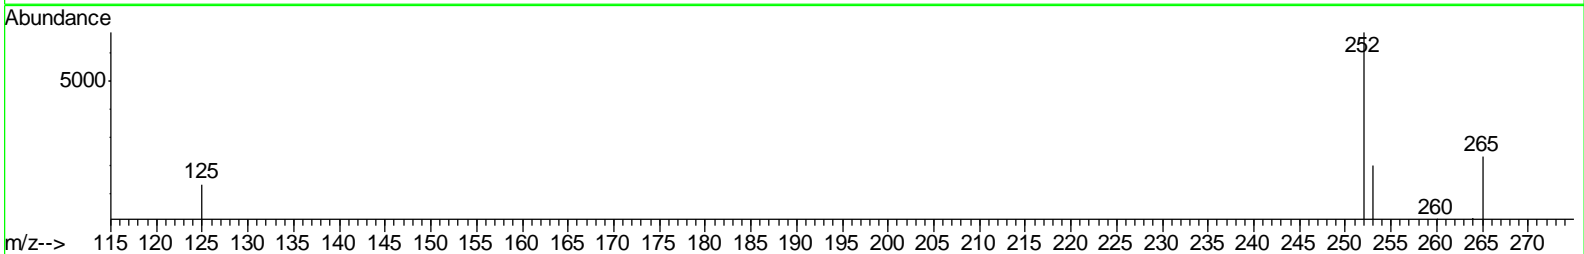


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012203.D
 Acq On : 14 Oct 2020 20:19
 Operator : CG/JU
 Sample : L4166-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Quant Time: Oct 15 01:06:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 00:46:15 2020
 Response via : Initial Calibration

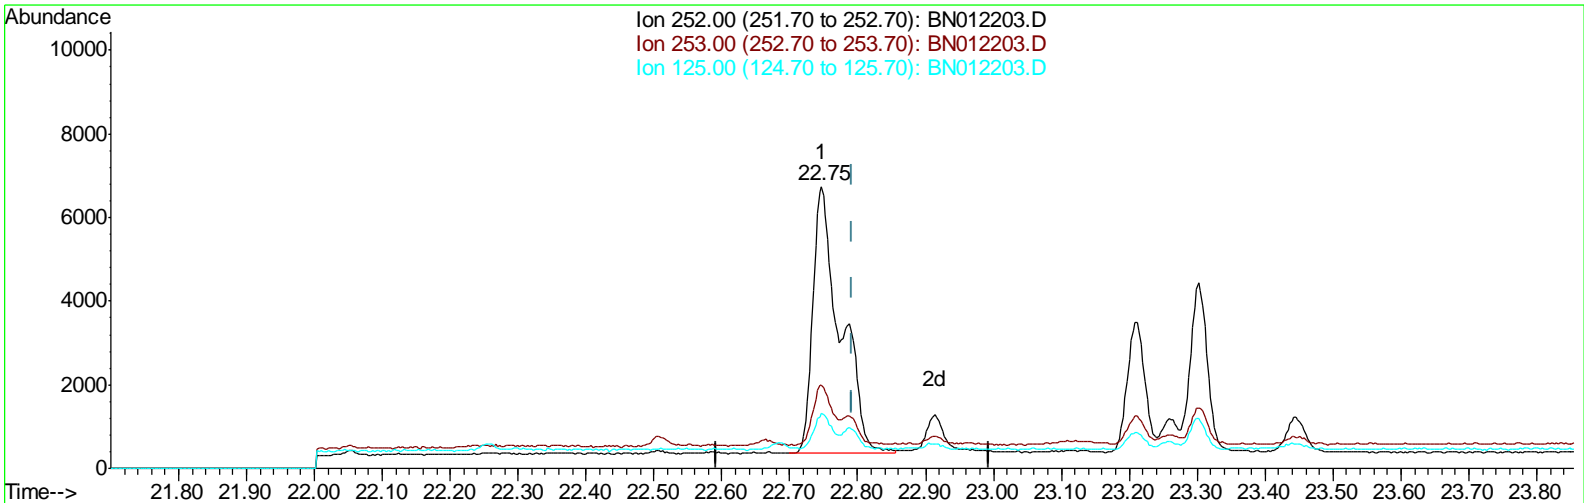

TIC: BN012203.D

(22) Benzo(k)fluoranthene
 22.747min (-0.047) 0.59ng/ul
 response 17917

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	29.56
125.00	16.10	19.47#
0.00	0.00	0.00