
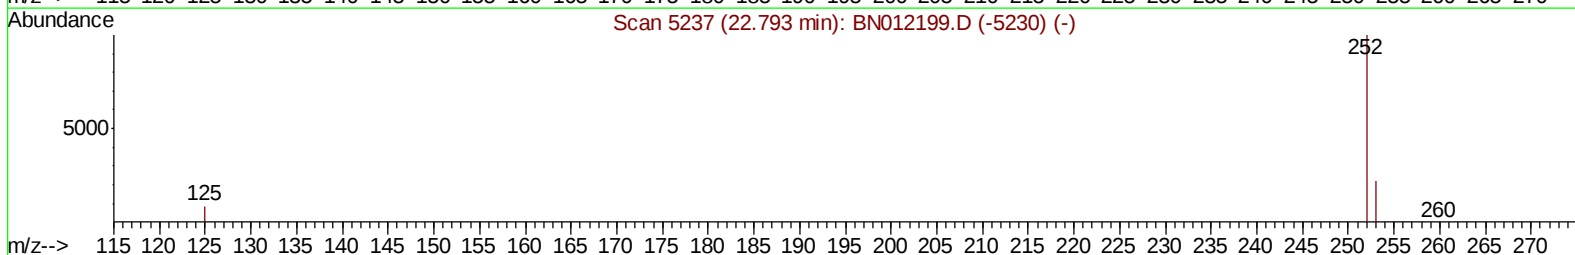
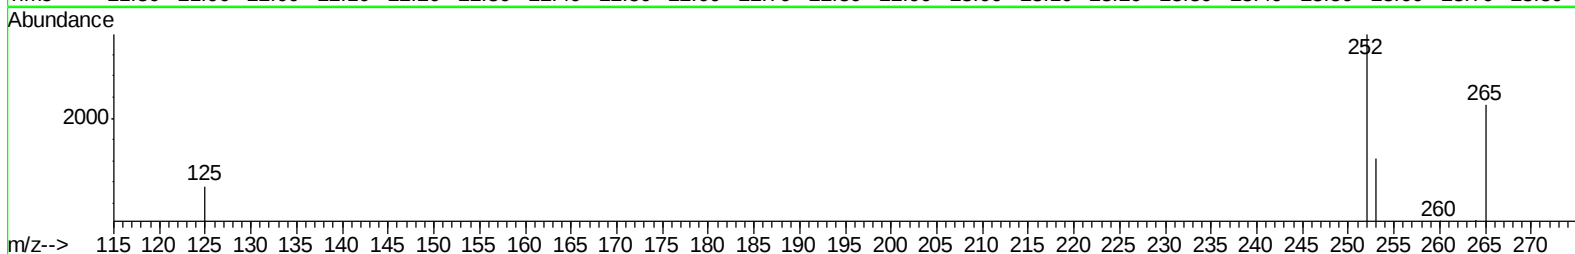


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012206.D
Acq On : 14 Oct 2020 22:07
Operator : CG/JU
Sample : L4166-07
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 15 00:54:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

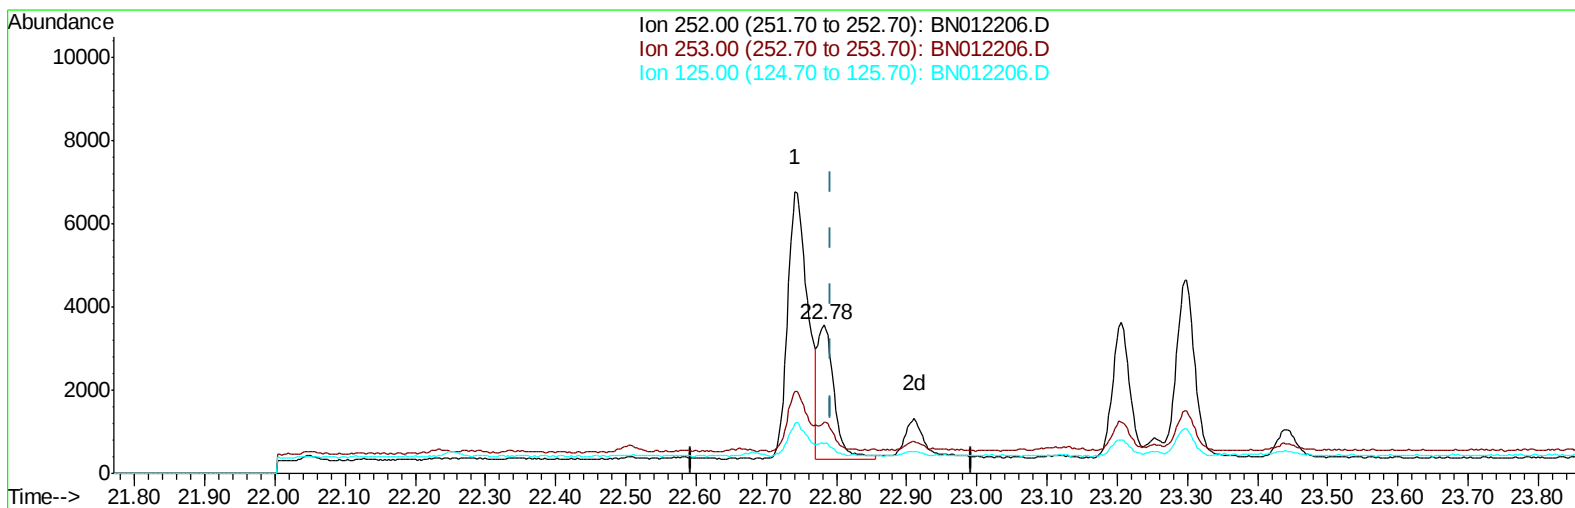

TIC: BN012206.D

(22) Benzo(k)fluoranthene

22.782min (-0.012) 0.24ng/ul m

response 5281

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	34.50
125.00	16.10	20.03#
0.00	0.00	0.00