
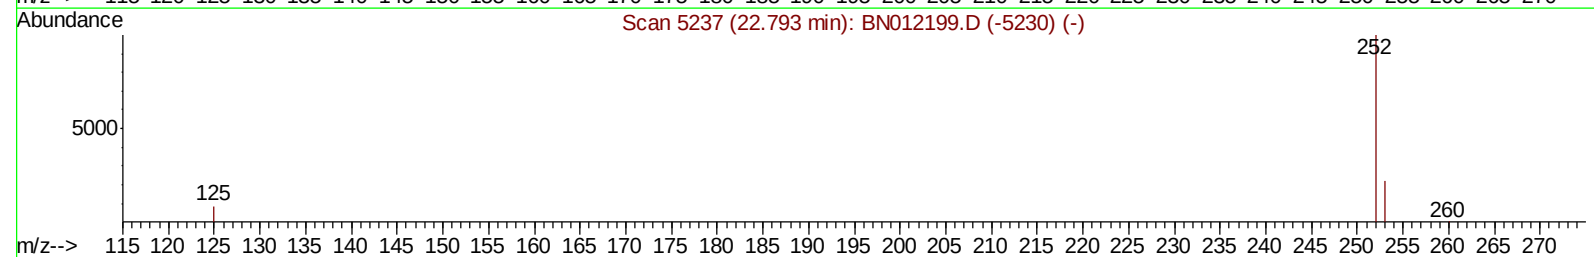
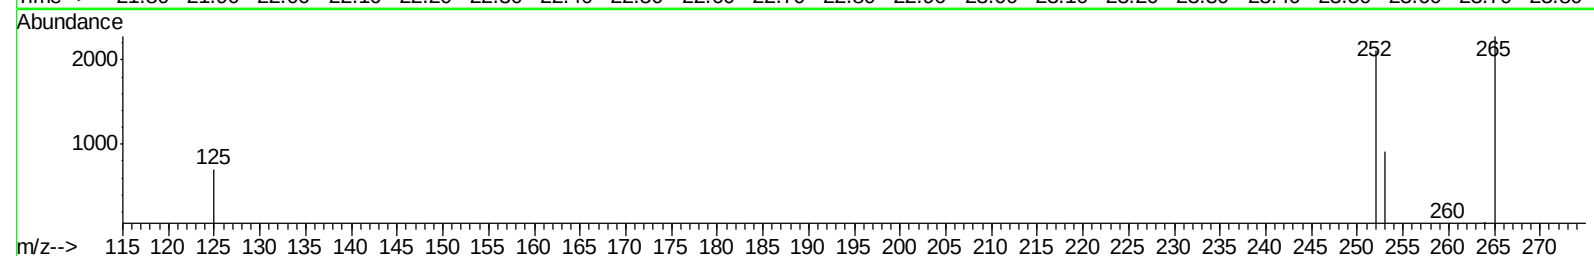


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012208.D
Acq On : 14 Oct 2020 23:19
Operator : CG/JU
Sample : L4166-08DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Oct 15 00:54:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

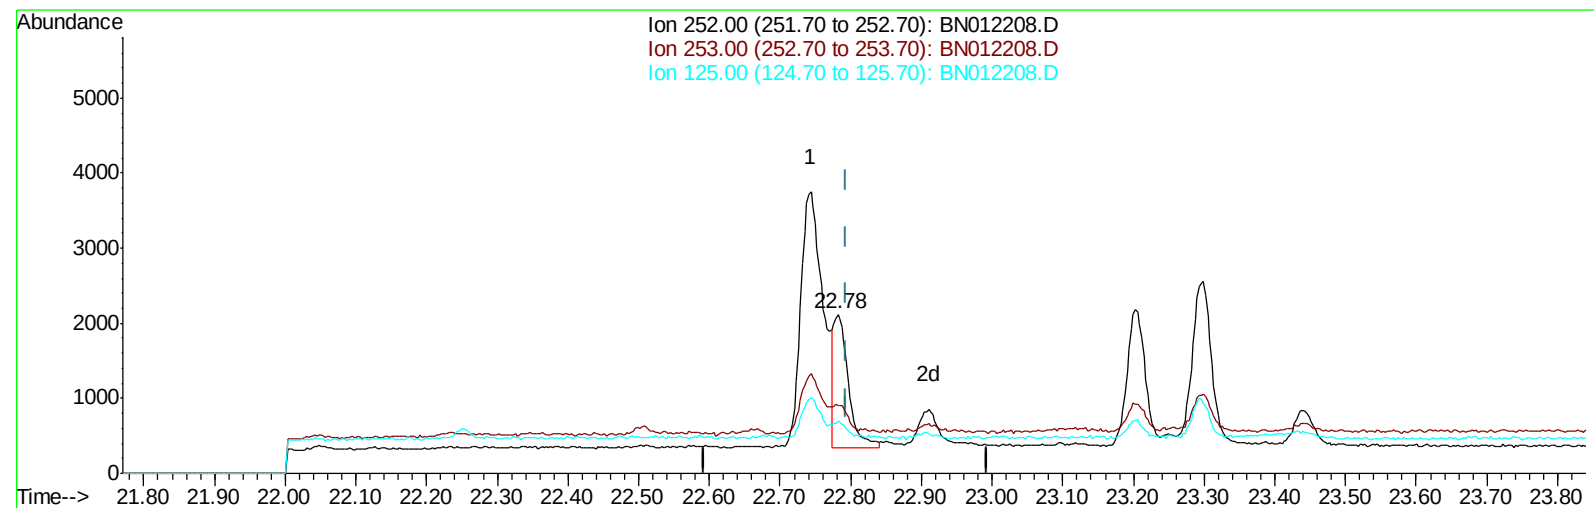

TIC: BN012208.D

(22) Benzo(k)fluoranthene

22.782min (-0.012) 0.09ng/ul m

response 2623

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	43.12#
125.00	16.10	32.77#
0.00	0.00	0.00