
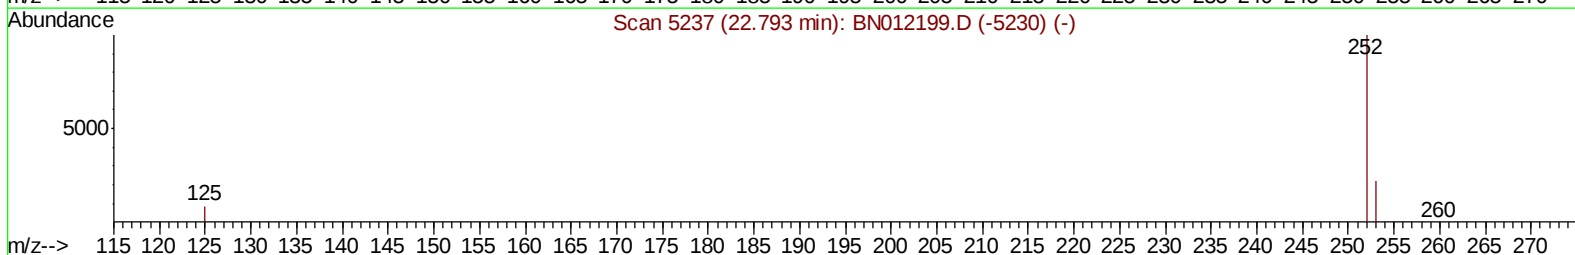
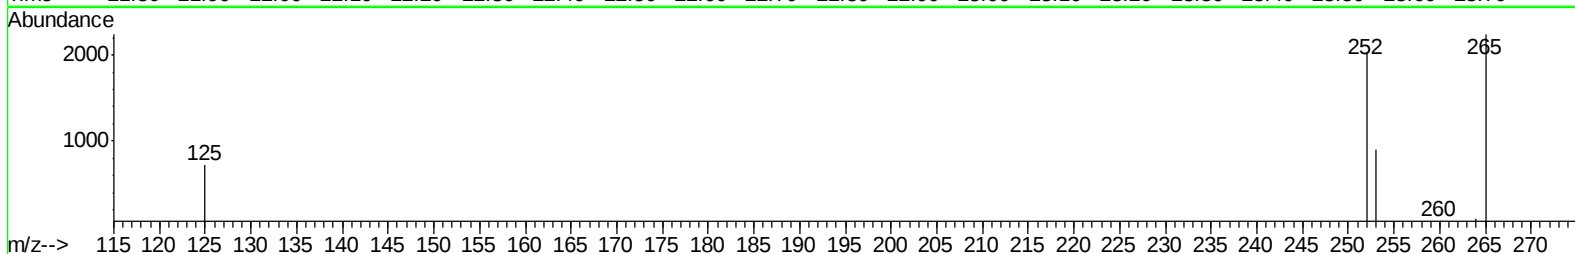


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012209.D
Acq On : 14 Oct 2020 23:56
Operator : CG/JU
Sample : L4166-06
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 15 01:26:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

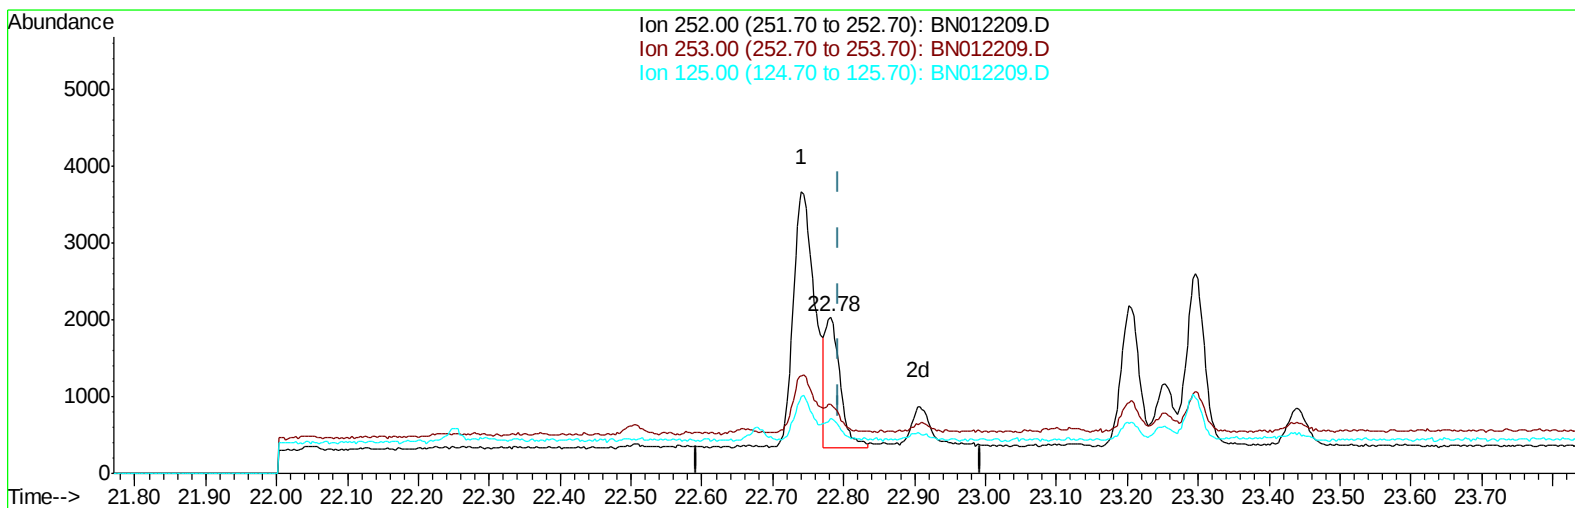

TIC: BN012209.D

(22) Benzo(k)fluoranthene

22.782min (-0.012) 0.11ng/ul m

response 2604

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	44.52#
125.00	16.10	35.33#
0.00	0.00	0.00