
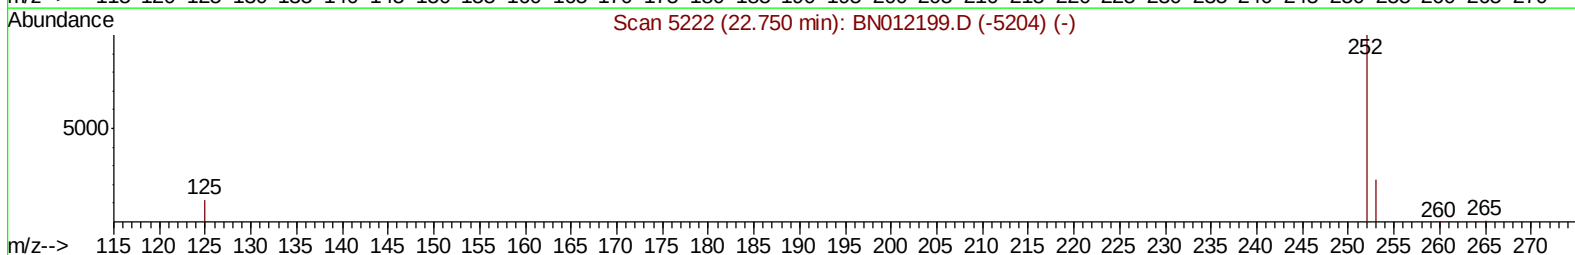
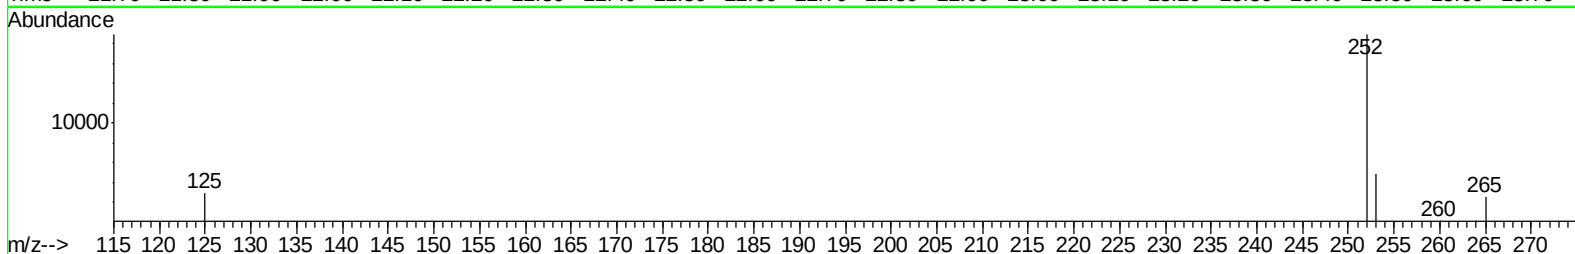


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012210.D
Acq On : 15 Oct 2020 00:32
Operator : CG/JU
Sample : L4166-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 15 02:13:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

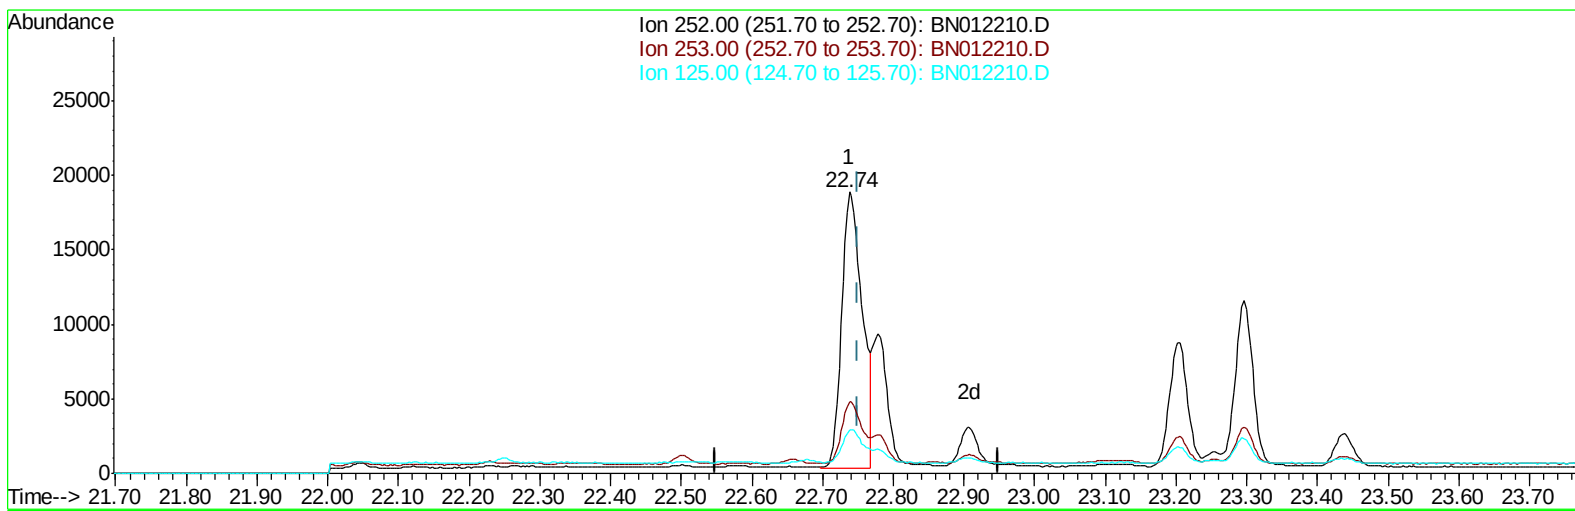

TIC: BN012210.D

(21) Benzo(b)fluoranthene

22.738min (-0.012) 1.36ng/ul m

response 37182

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	25.38
125.00	18.40	15.27
0.00	0.00	0.00