
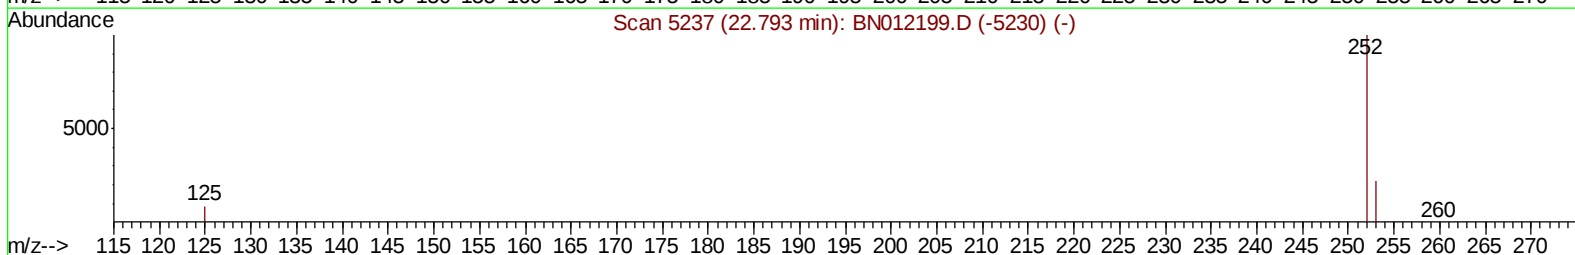
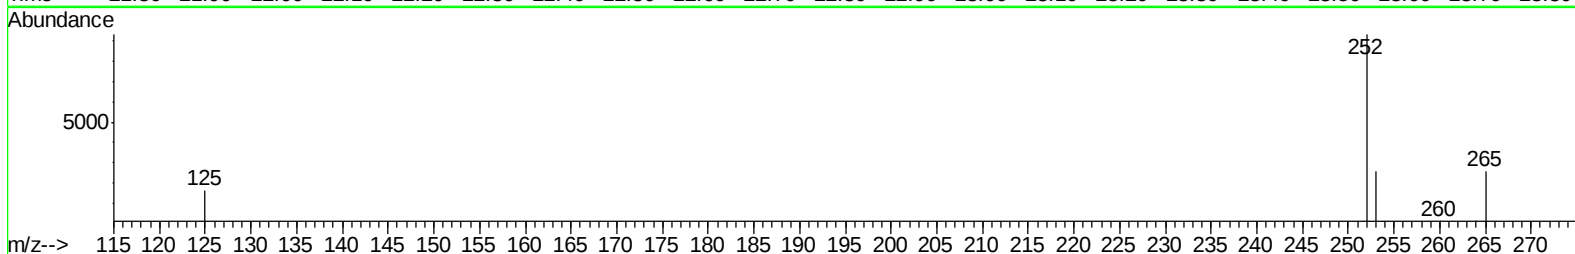


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012210.D
 Acq On : 15 Oct 2020 00:32
 Operator : CG/JU
 Sample : L4166-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Quant Time: Oct 15 02:13:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 00:46:15 2020
 Response via : Initial Calibration

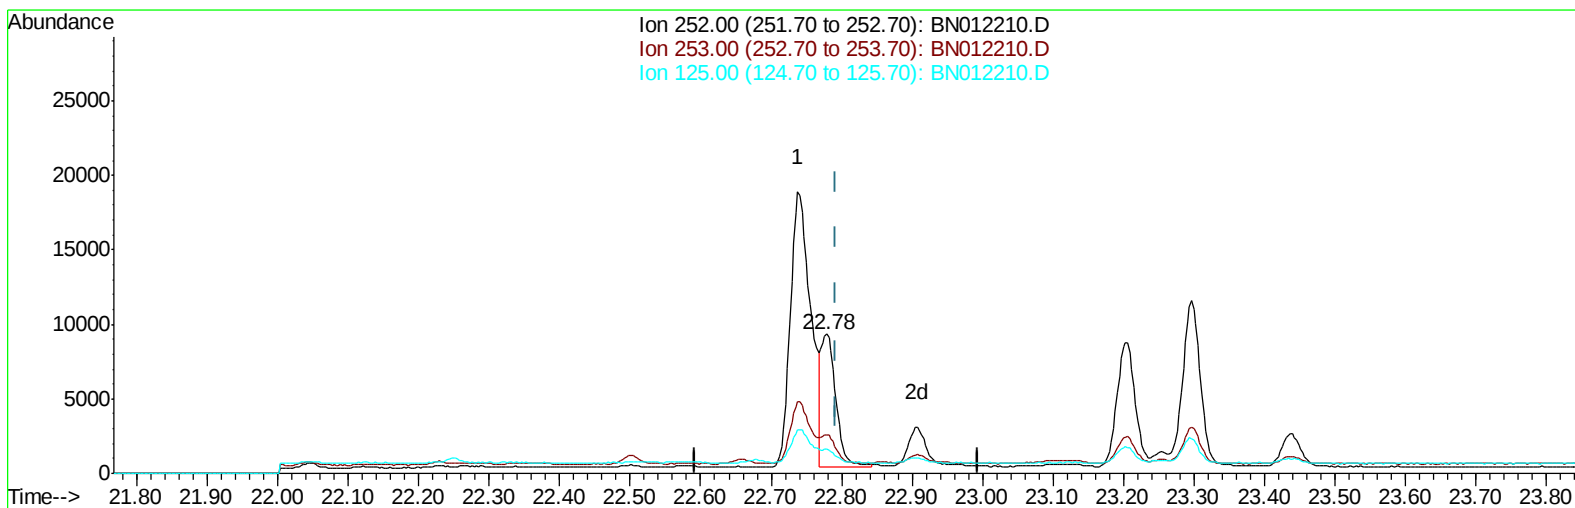

TIC: BN012210.D

(22) Benzo(k)fluoranthene

22.779min (-0.015) 0.45ng/ul m

response 13515

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.70
125.00	16.10	17.04
0.00	0.00	0.00