
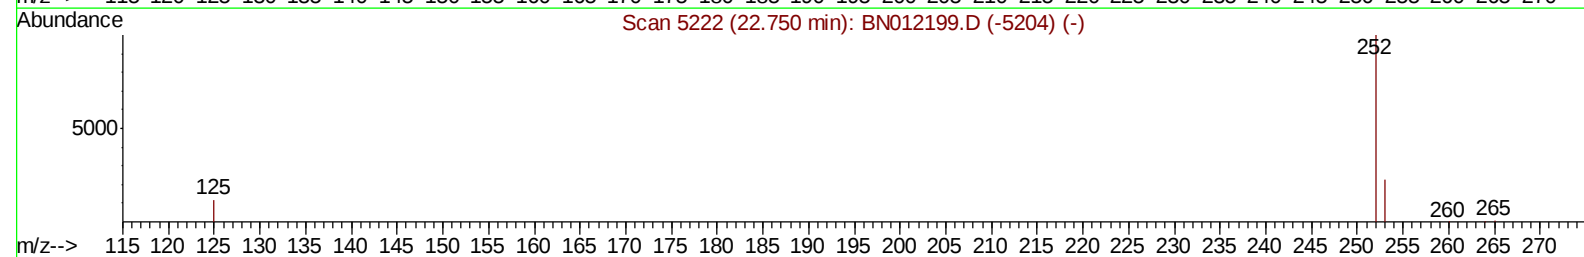
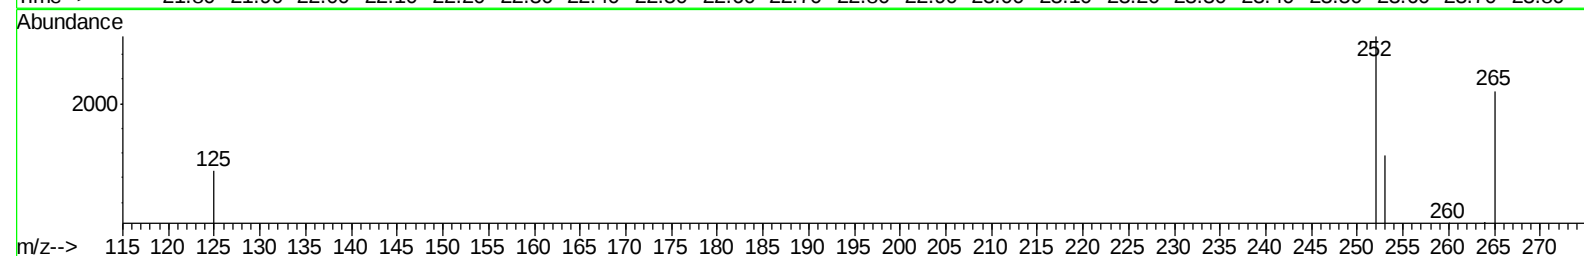


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012211.D
 Acq On : 15 Oct 2020 01:08
 Operator : CG/JU
 Sample : L4166-10DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 15 01:51:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 00:46:15 2020
 Response via : Initial Calibration

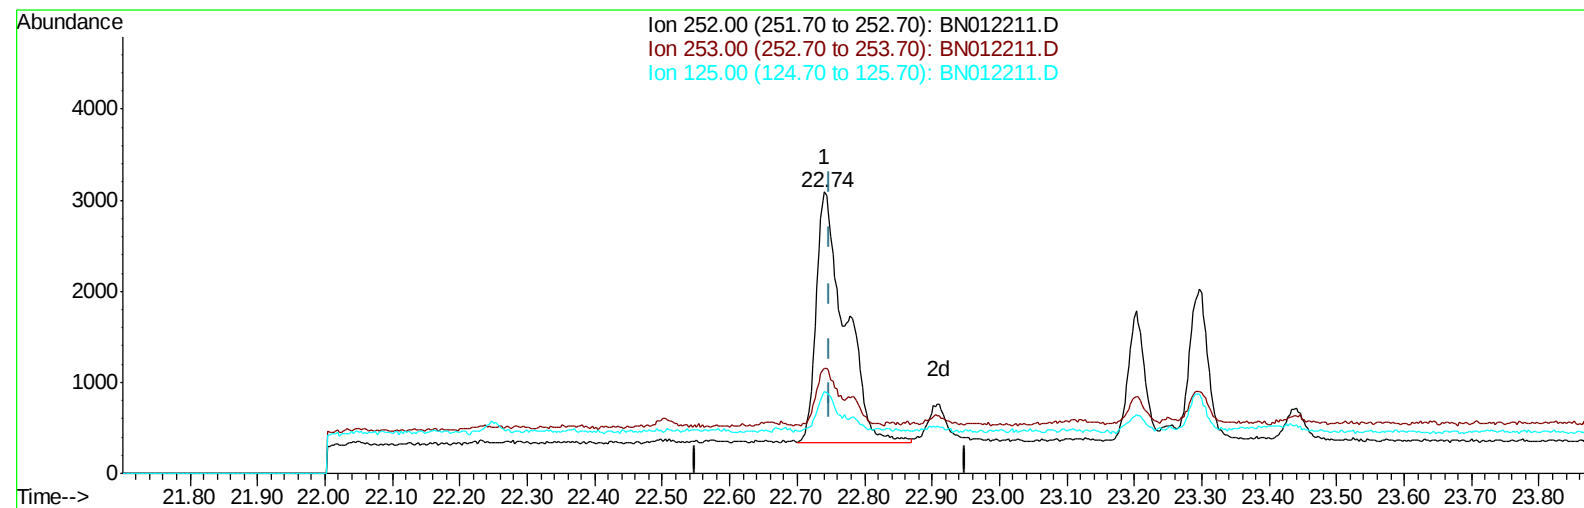

TIC: BN012211.D

(21) Benzo(b)fluoranthene
 22.741min (-0.009) 0.28ng/ul
 response 8138

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	37.32
125.00	18.40	29.24
0.00	0.00	0.00