
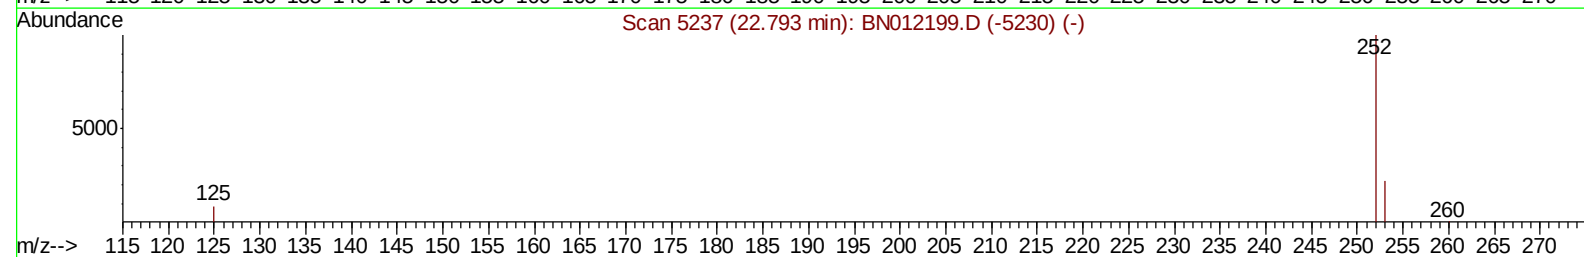
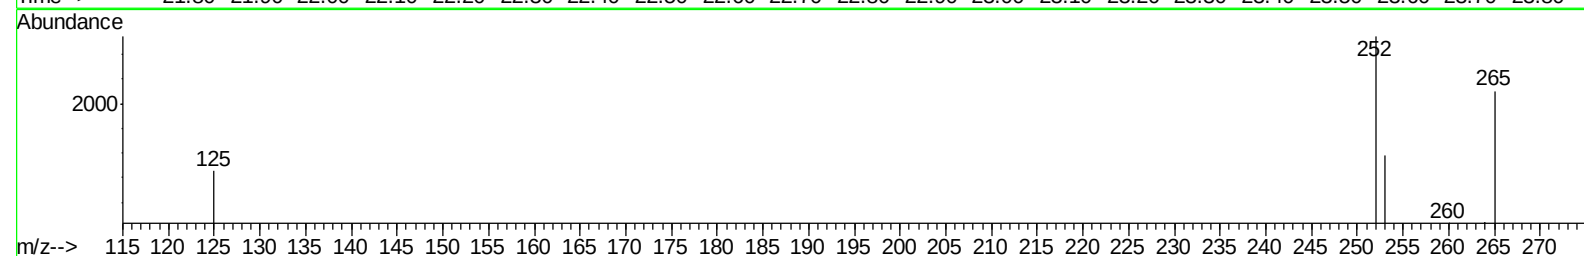


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012211.D
 Acq On : 15 Oct 2020 01:08
 Operator : CG/JU
 Sample : L4166-10DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Quant Time: Oct 15 01:51:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 00:46:15 2020
 Response via : Initial Calibration

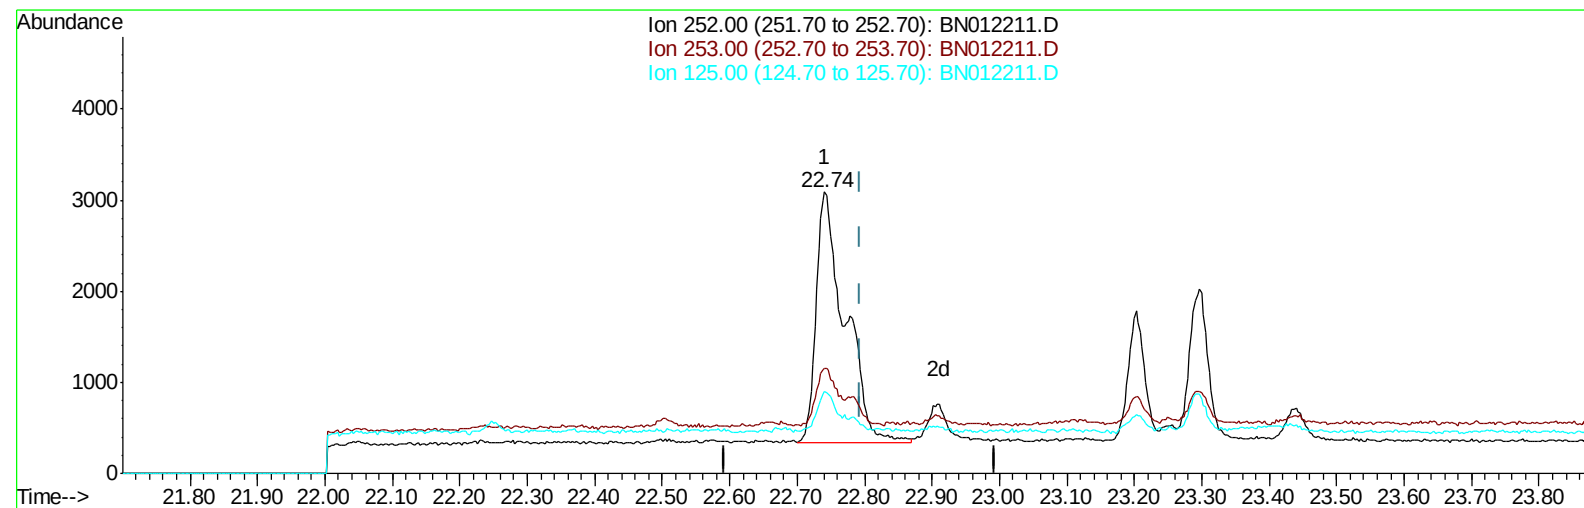

TIC: BN012211.D

(22) Benzo(k)fluoranthene

22.741min (-0.053) 0.25ng/ul

response 8138

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	37.32#
125.00	16.10	29.24#
0.00	0.00	0.00