
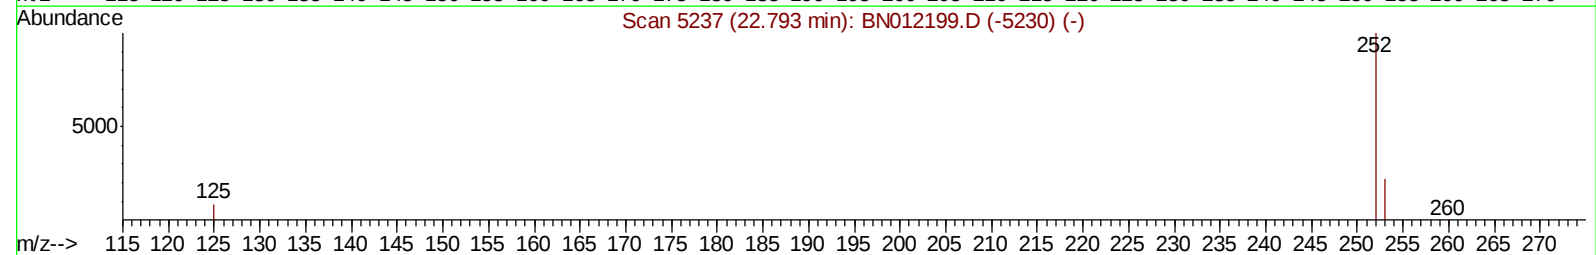
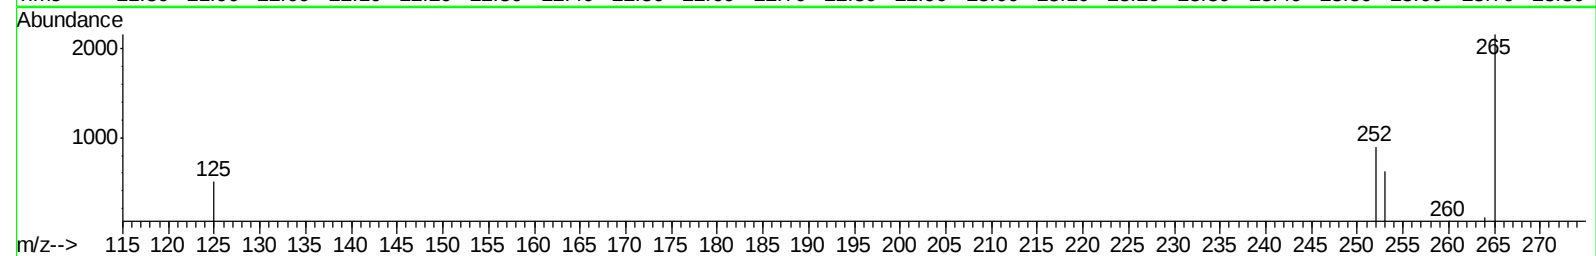


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012212.D
Acq On : 15 Oct 2020 01:44
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Oct 15 02:25:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

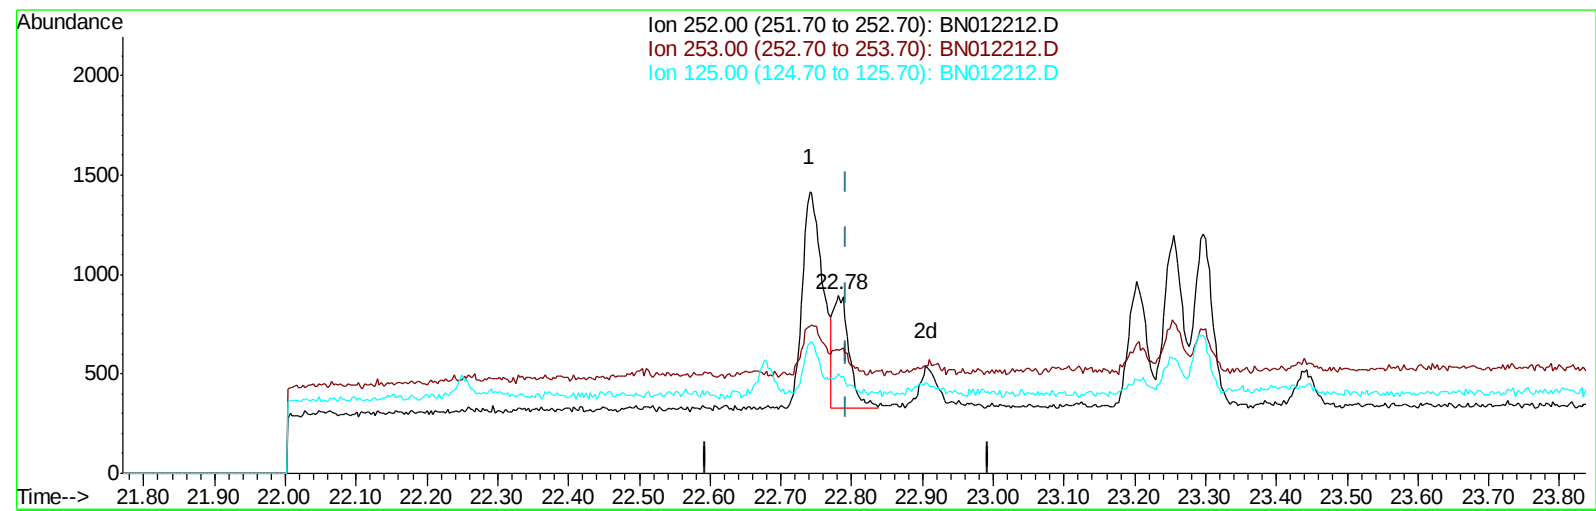

TIC: BN012212.D

(22) Benzo(k)fluoranthene

22.782min (-0.012) 0.03ng/ul m

response 909

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	69.16#
125.00	16.10	56.09#
0.00	0.00	0.00