
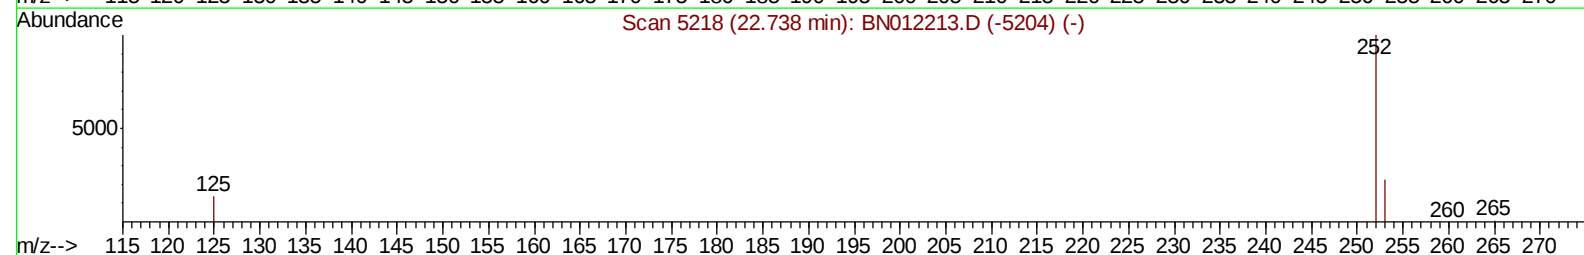
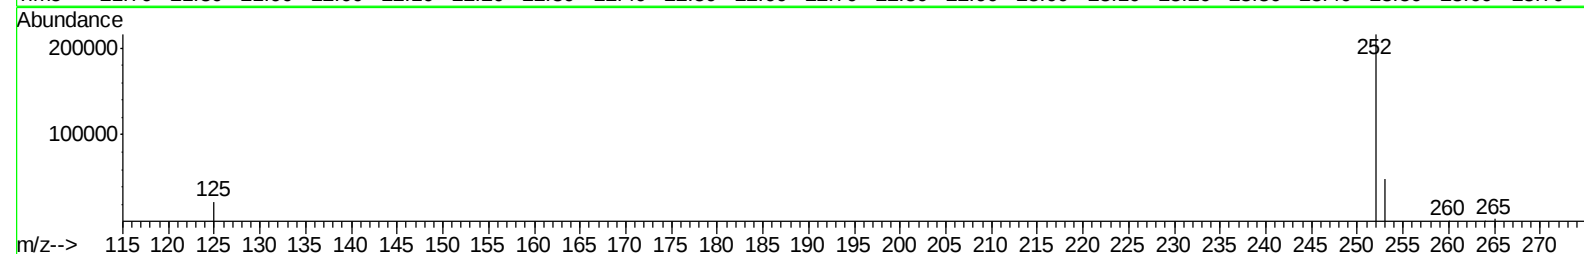


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012215.D
Acq On : 15 Oct 2020 04:10
Operator : CG/JU
Sample : L4184-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Oct 15 04:55:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

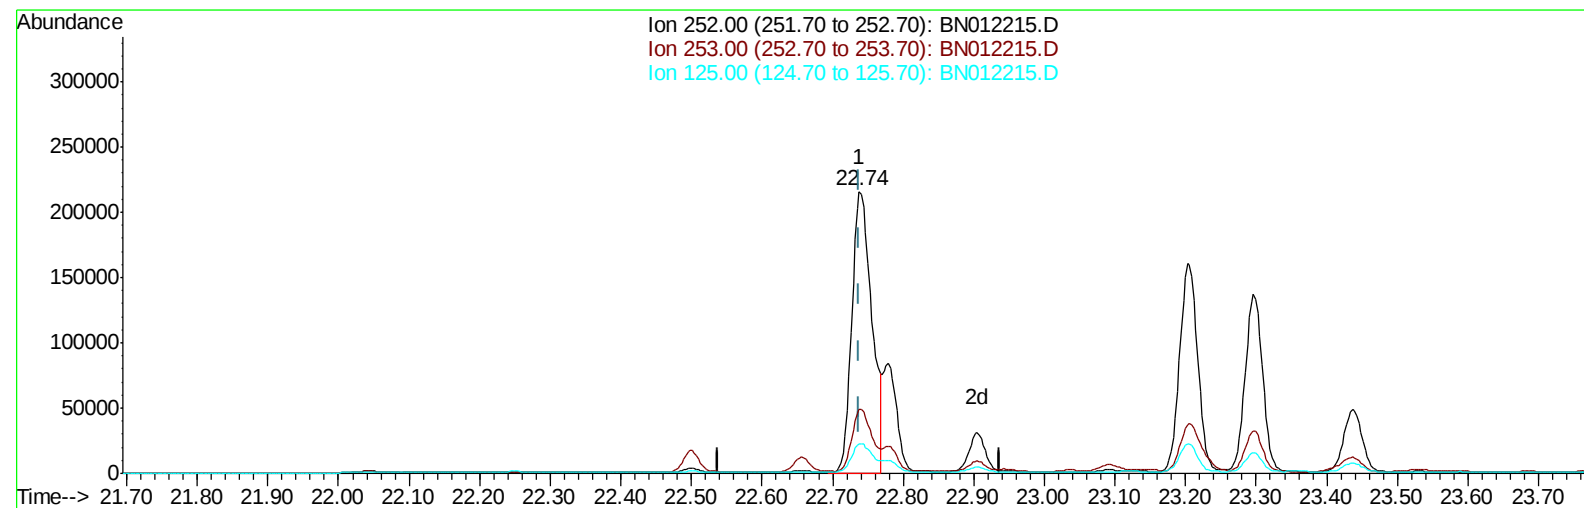

TIC: BN012215.D

(21) Benzo(b)fluoranthene

22.738min (0.000) 15.39ng/ul m

response 421373

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	22.80
125.00	18.40	10.59
0.00	0.00	0.00