
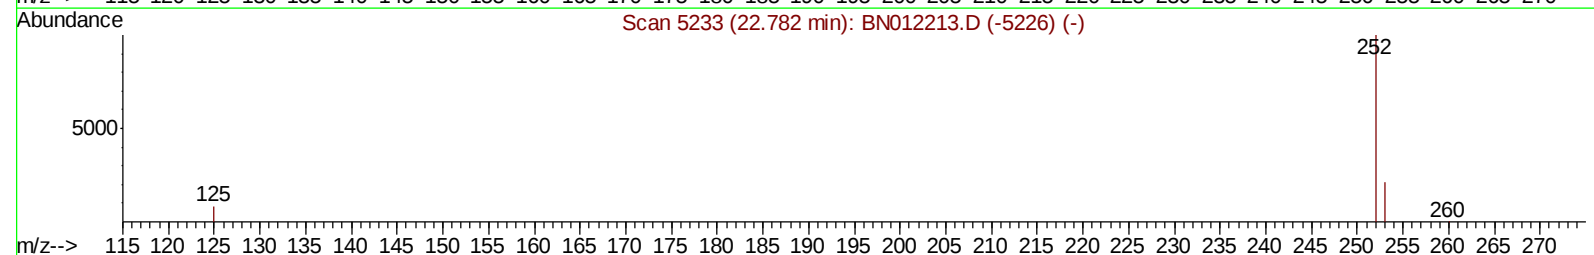
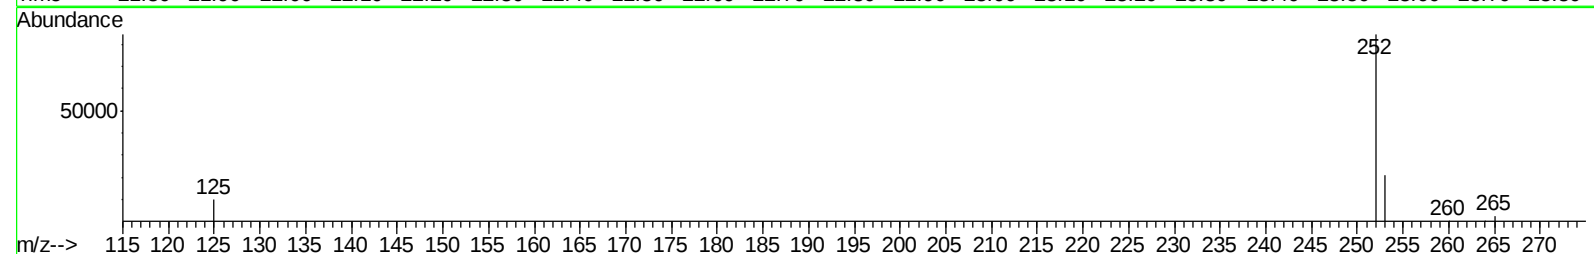


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012215.D
 Acq On : 15 Oct 2020 04:10
 Operator : CG/JU
 Sample : L4184-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Oct 15 04:55:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 04:47:44 2020
 Response via : Initial Calibration

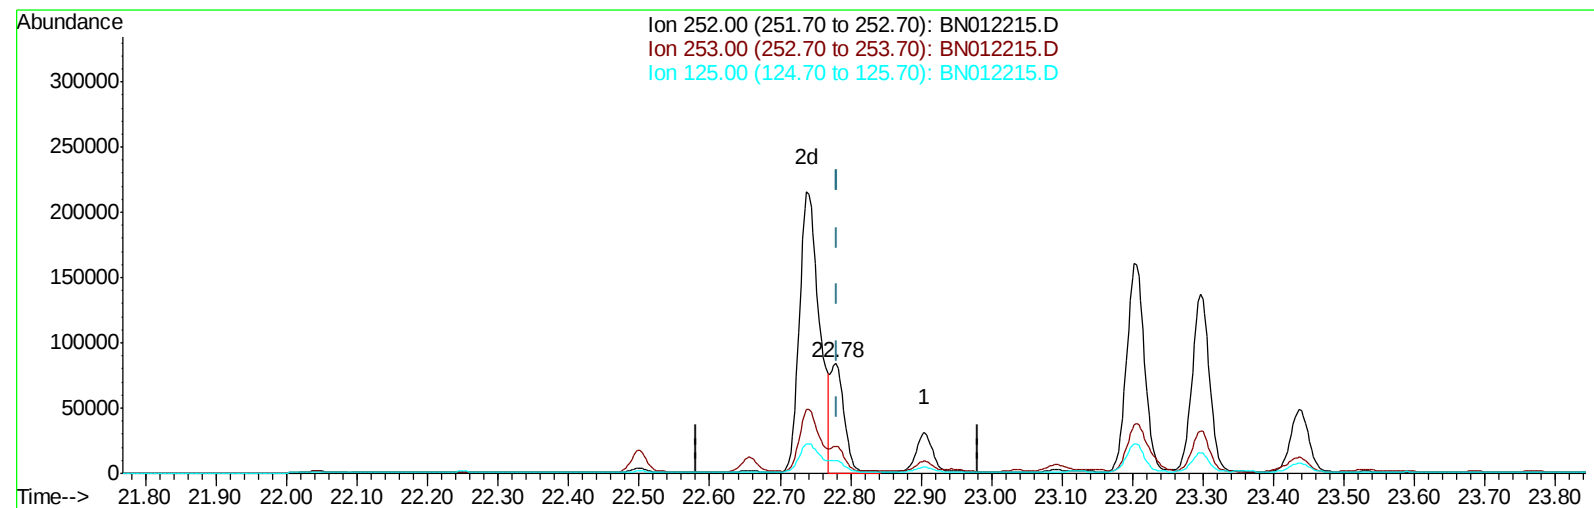

TIC: BN012215.D

(22) Benzo(k)fluoranthene

22.779min (-0.003) 3.98ng/ul m

response 120510

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	24.94
125.00	16.10	11.77#
0.00	0.00	0.00