
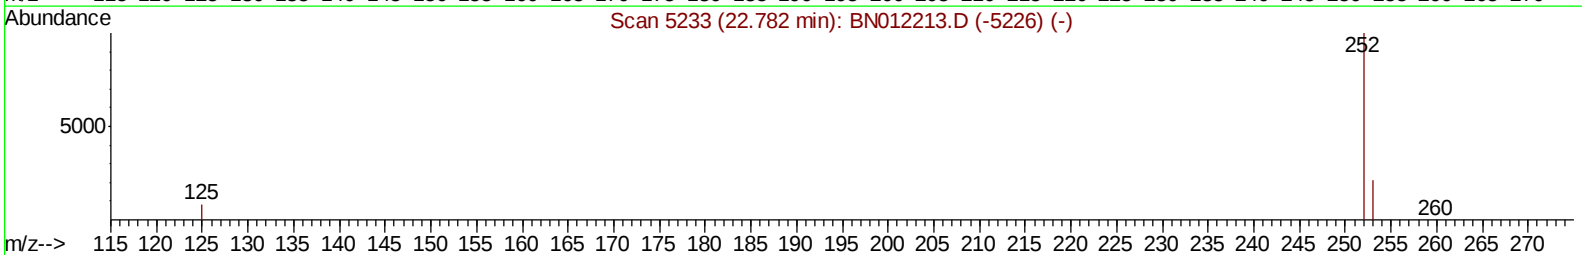
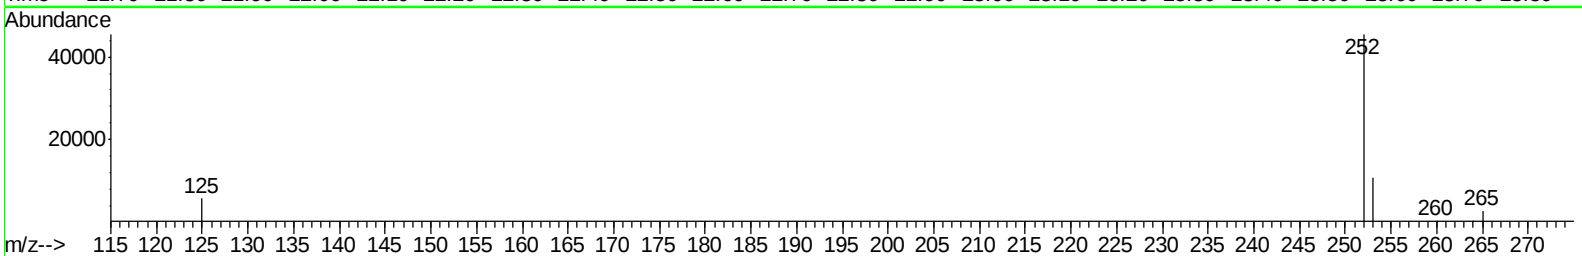


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012216.D
Acq On : 15 Oct 2020 04:46
Operator : CG/JU
Sample : L4184-12DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Oct 15 07:16:54 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

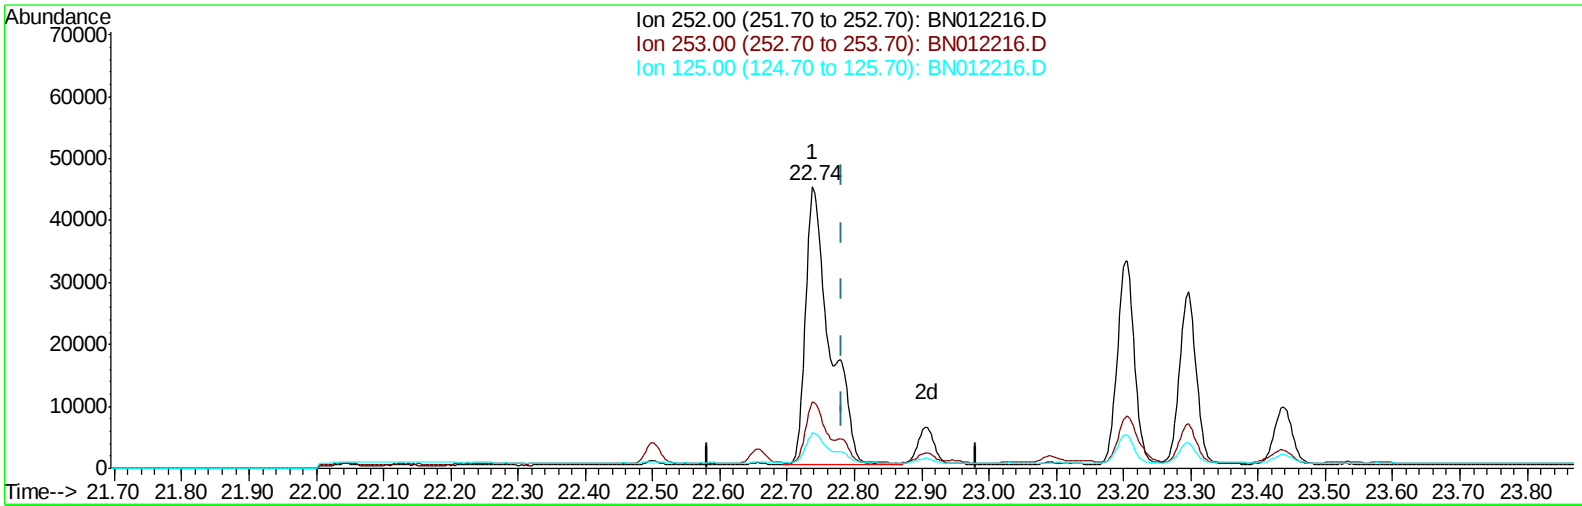

TIC: BN012216.D

(22) Benzo(k)fluoranthene
22.738min (-0.044) 3.31ng/ul
response 112310

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	23.85#
125.00	16.10	12.56#
0.00	0.00	0.00