
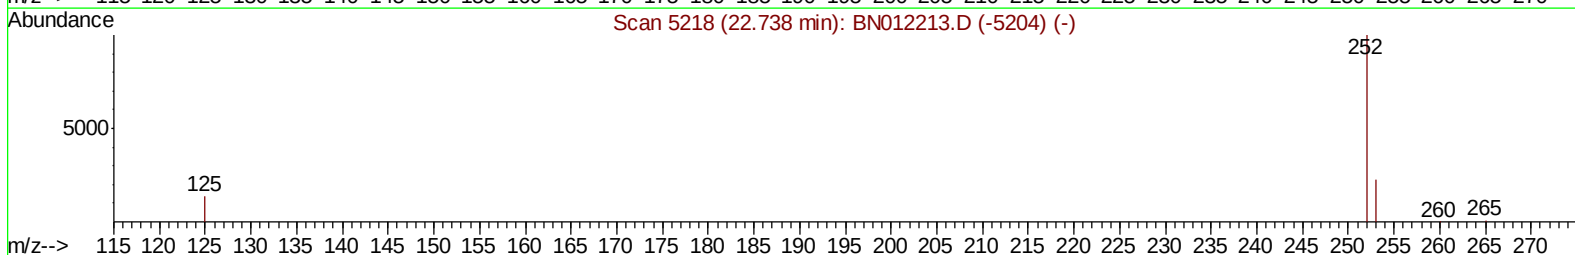
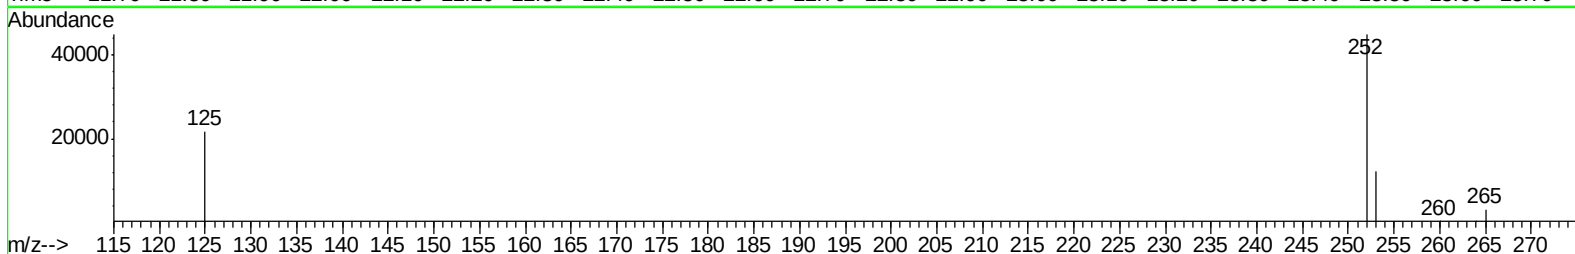


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012217.D
Acq On : 15 Oct 2020 05:22
Operator : CG/JU
Sample : L4184-20
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Oct 15 07:28:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

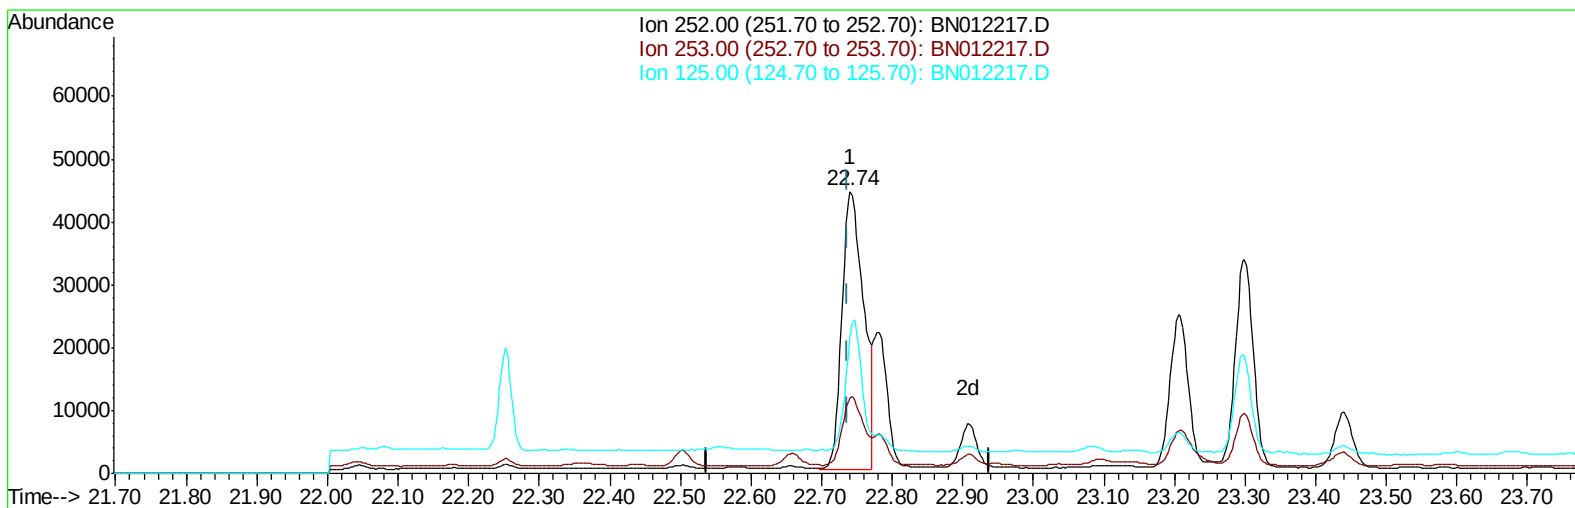

TIC: BN012217.D

(21) Benzo(b)fluoranthene

22.741min (+0.003) 3.48ng/ul m

response 93438

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	27.06
125.00	18.40	48.46#
0.00	0.00	0.00