
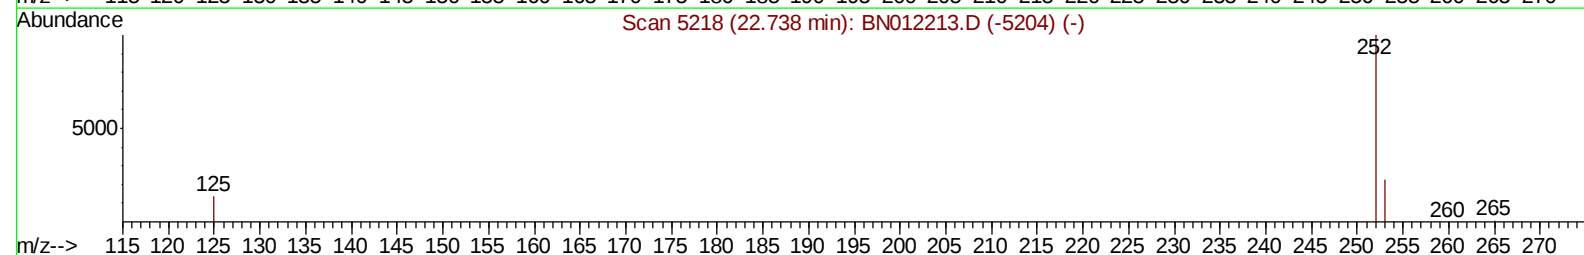
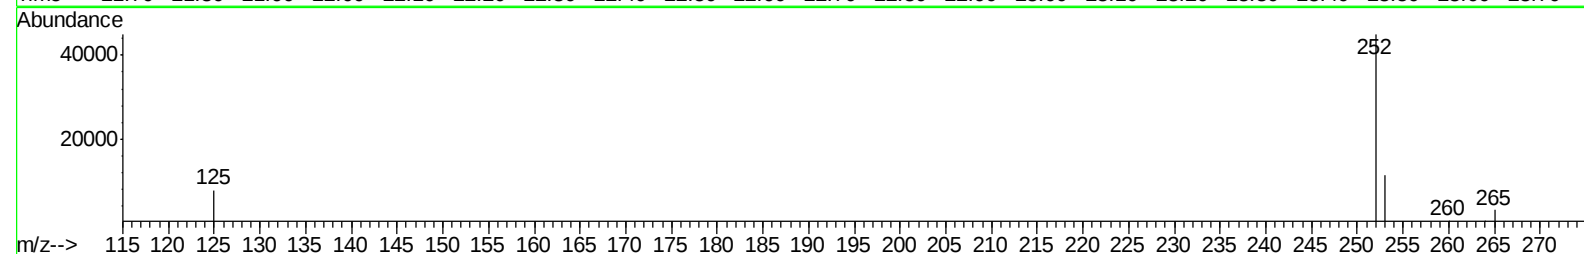


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012218.D
Acq On : 15 Oct 2020 05:57
Operator : CG/JU
Sample : L4184-15DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 15 07:17:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

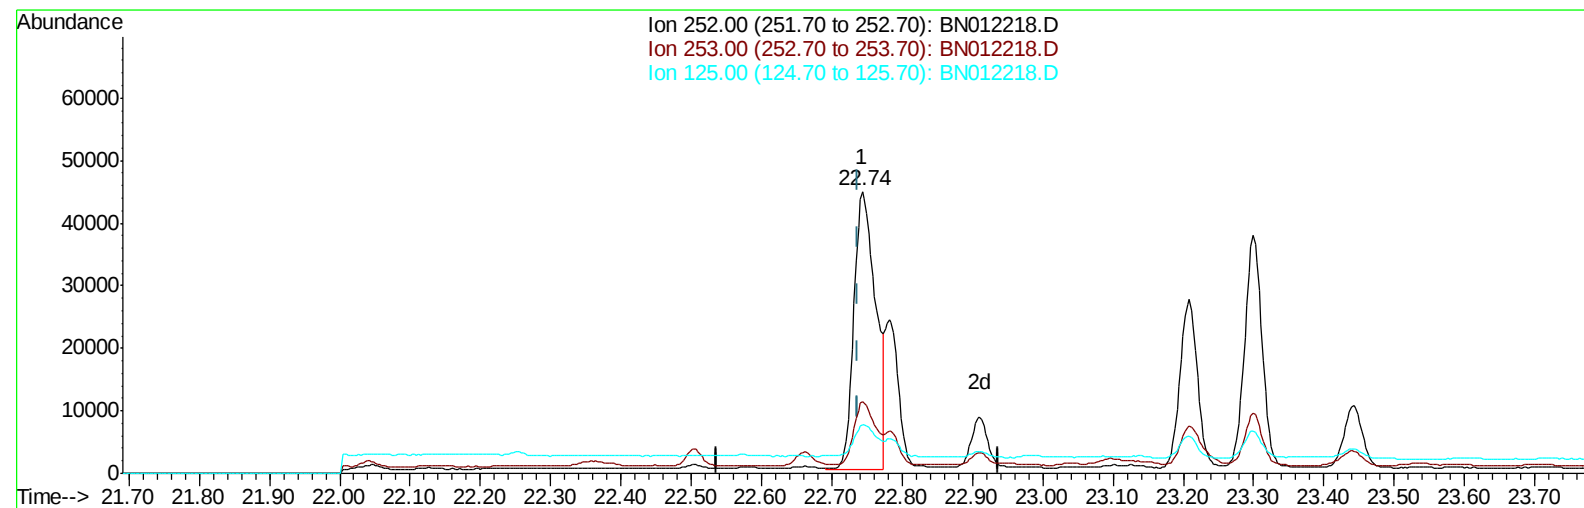

TIC: BN012218.D

(21) Benzo(b)fluoranthene

22.744min (+0.006) 2.66ng/ul m

response 95588

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	25.48
125.00	18.40	17.25
0.00	0.00	0.00