
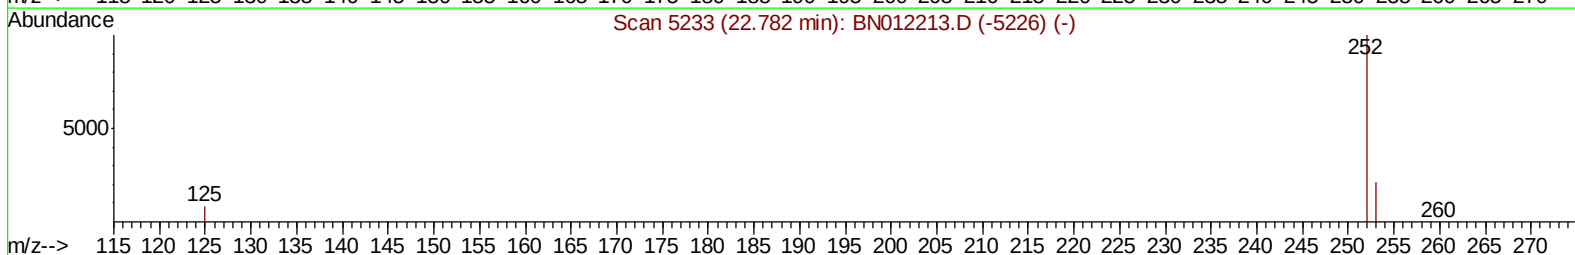
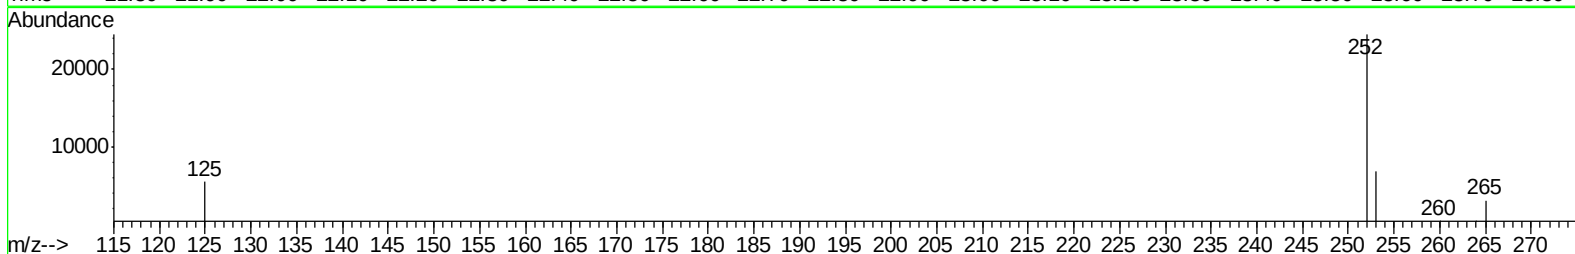


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012218.D
Acq On : 15 Oct 2020 05:57
Operator : CG/JU
Sample : L4184-15DL 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Quant Time: Oct 15 07:17:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

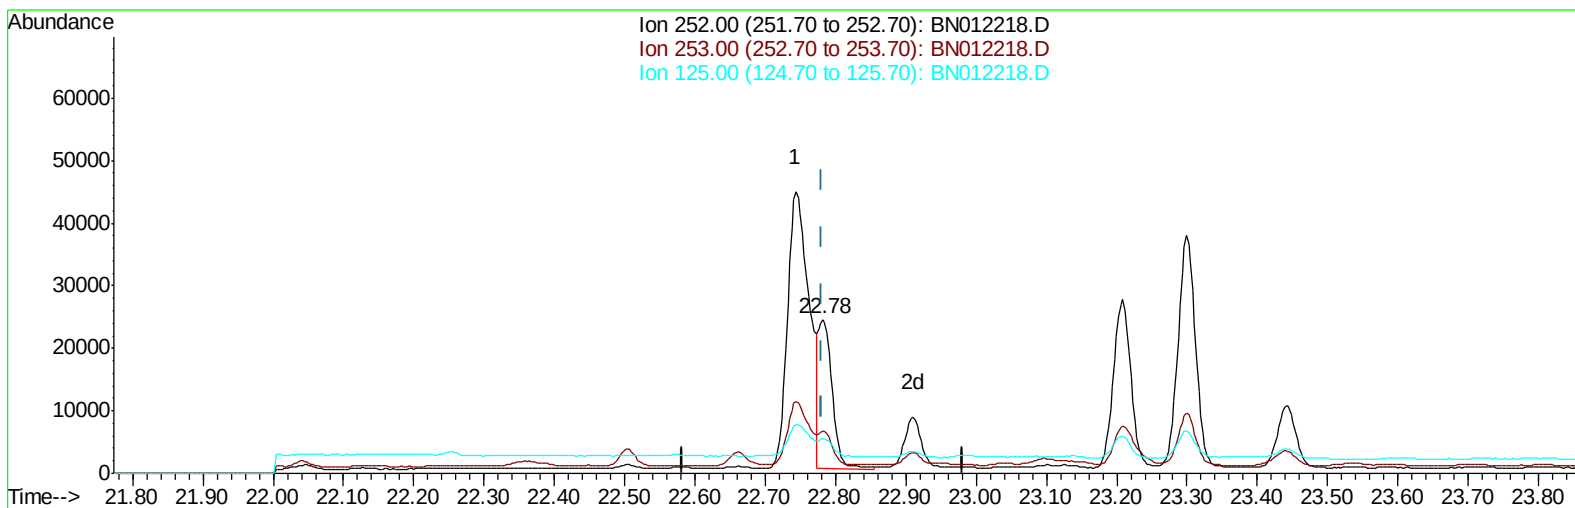

TIC: BN012218.D

(22) Benzo(k)fluoranthene

22.782min (-0.000) 0.83ng/ul m

response 32796

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.59
125.00	16.10	22.19#
0.00	0.00	0.00