
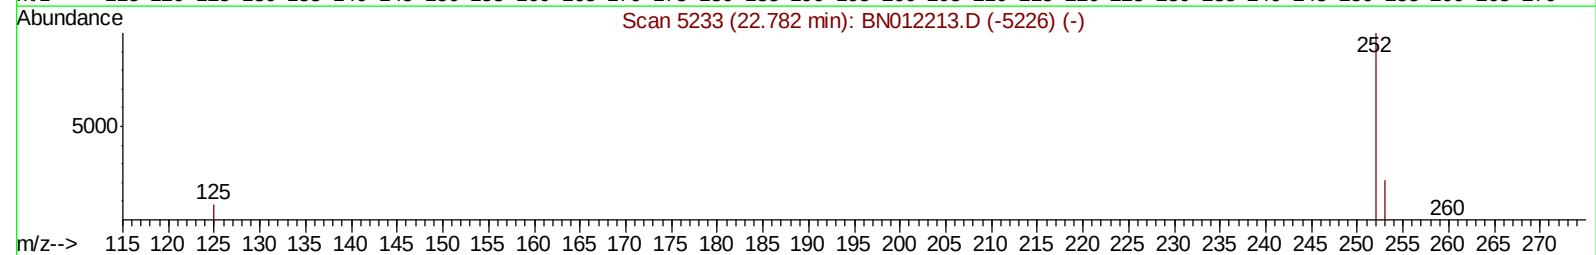
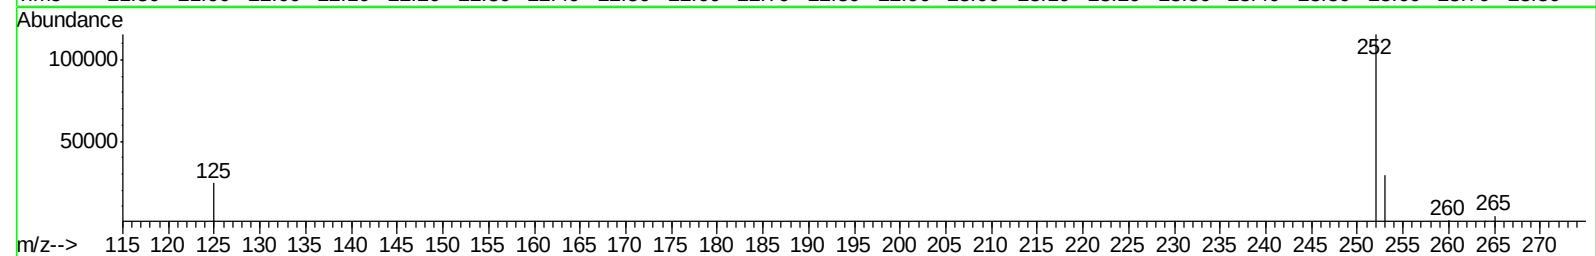


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012219.D
Acq On : 15 Oct 2020 06:34
Operator : CG/JU
Sample : L4184-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Oct 15 08:00:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

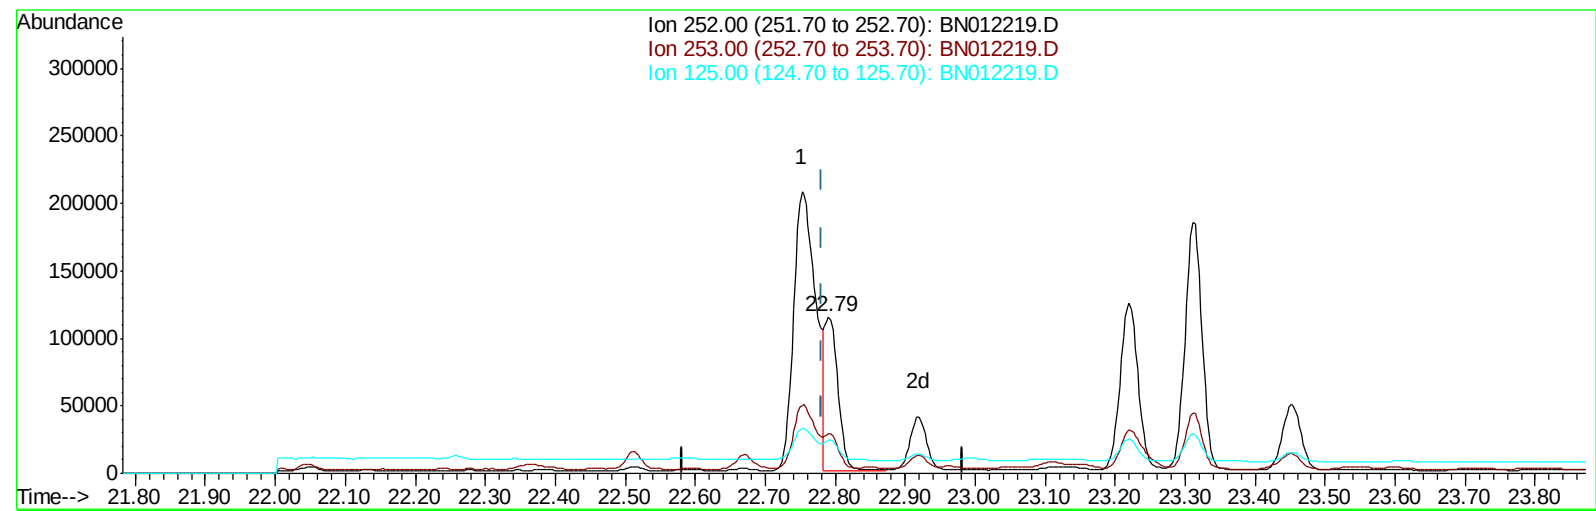

TIC: BN012219.D

(22) Benzo(k)fluoranthene

22.791min (+0.009) 5.06ng/ul m

response 155538

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	25.40
125.00	16.10	20.93#
0.00	0.00	0.00