
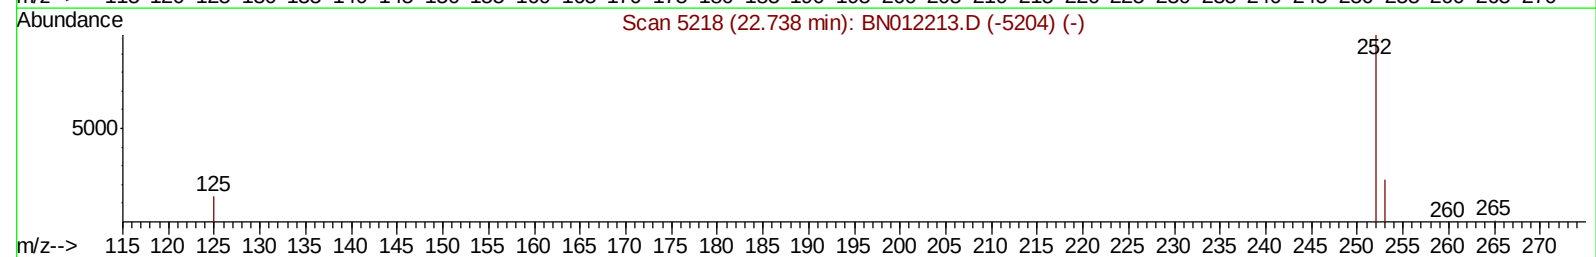
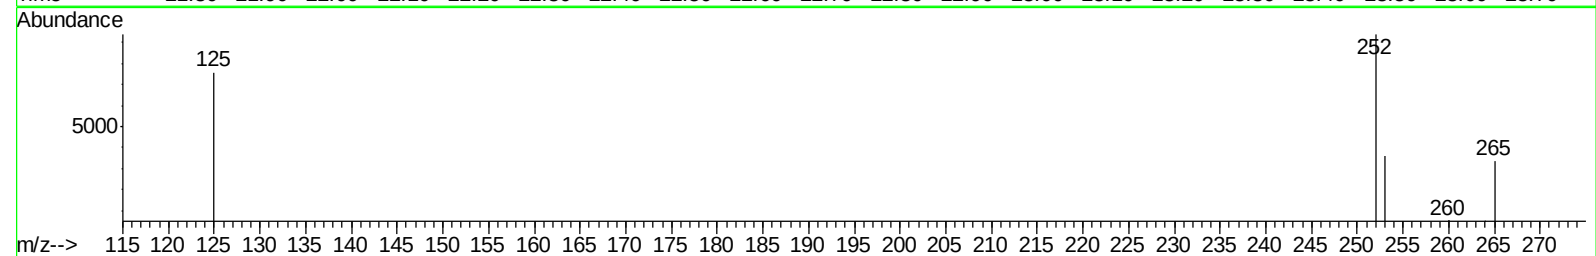


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012220.D
Acq On : 15 Oct 2020 07:10
Operator : CG/JU
Sample : L4184-20DL 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Oct 15 08:09:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

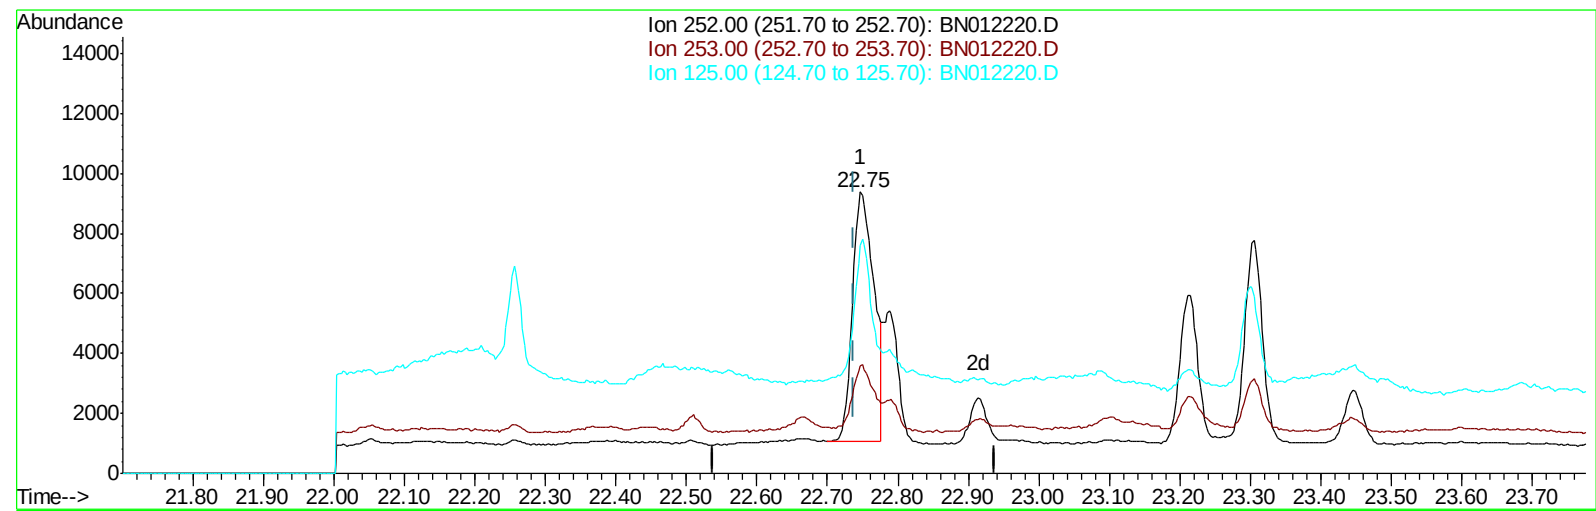

TIC: BN012220.D

(21) Benzo(b)fluoranthene

22.747min (+0.009) 0.45ng/ul m

response 17724

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	38.14
125.00	18.40	80.75#
0.00	0.00	0.00