
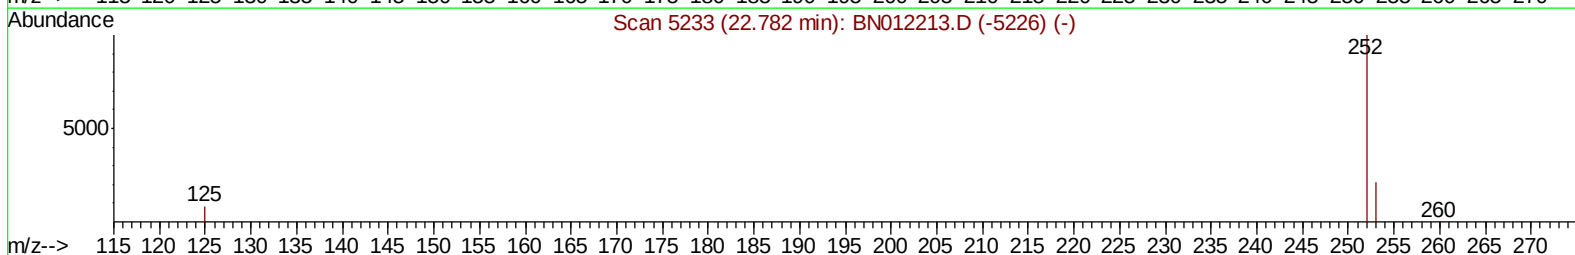
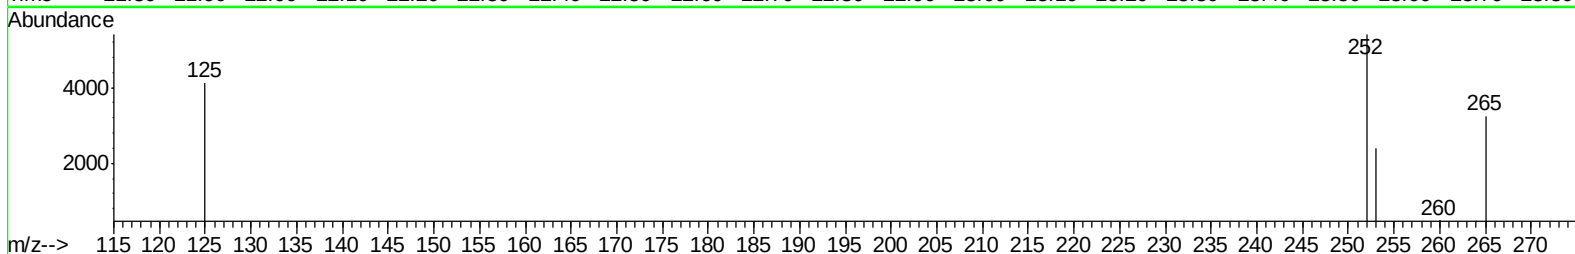


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012220.D
Acq On : 15 Oct 2020 07:10
Operator : CG/JU
Sample : L4184-20DL 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Oct 15 08:09:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 04:47:44 2020
Response via : Initial Calibration

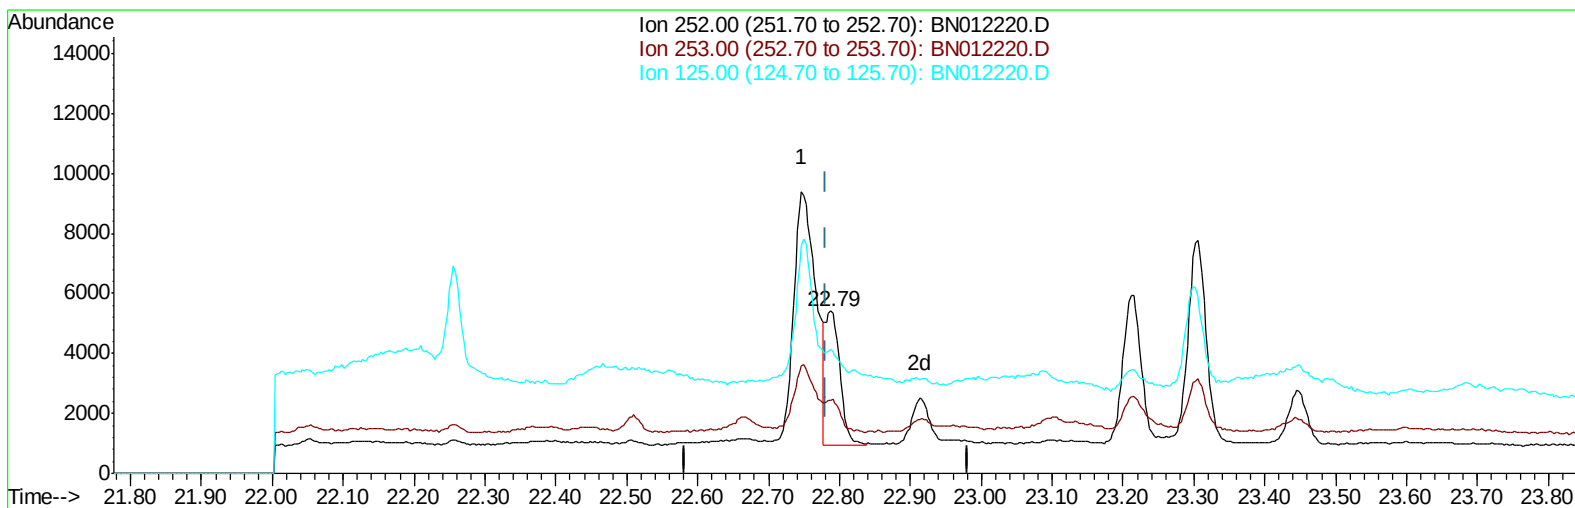

TIC: BN012220.D

(22) Benzo(k)fluoranthene

22.788min (+0.006) 0.15ng/ul m

response 6648

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	44.61#
125.00	16.10	76.37#
0.00	0.00	0.00