
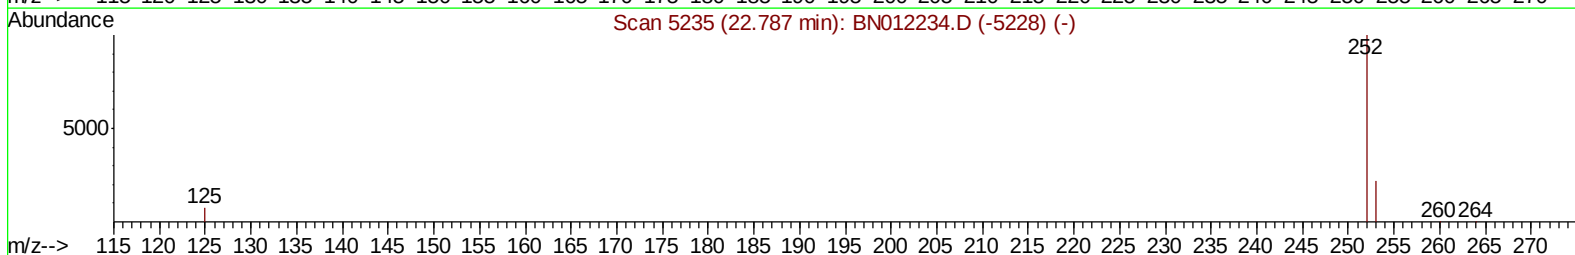
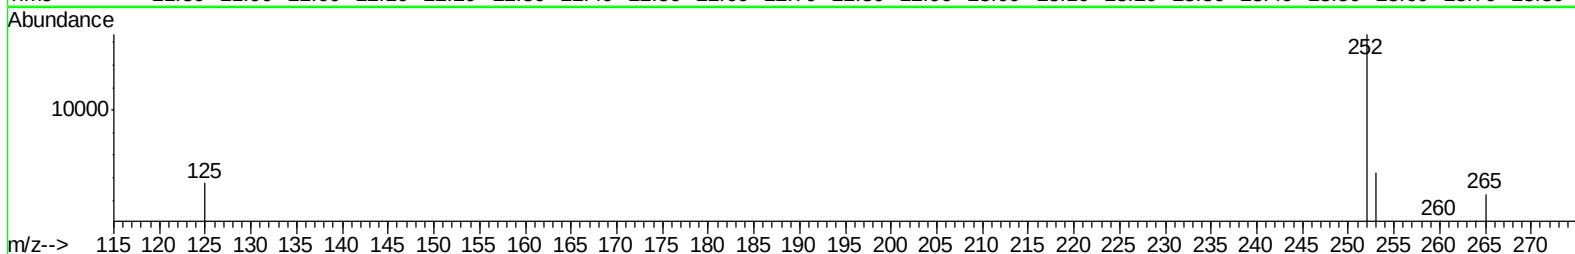


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012238.D
 Acq On : 15 Oct 2020 19:12
 Operator : CG/JU
 Sample : L4235-03
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Quant Time: Oct 16 01:27:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:19:50 2020
 Response via : Initial Calibration

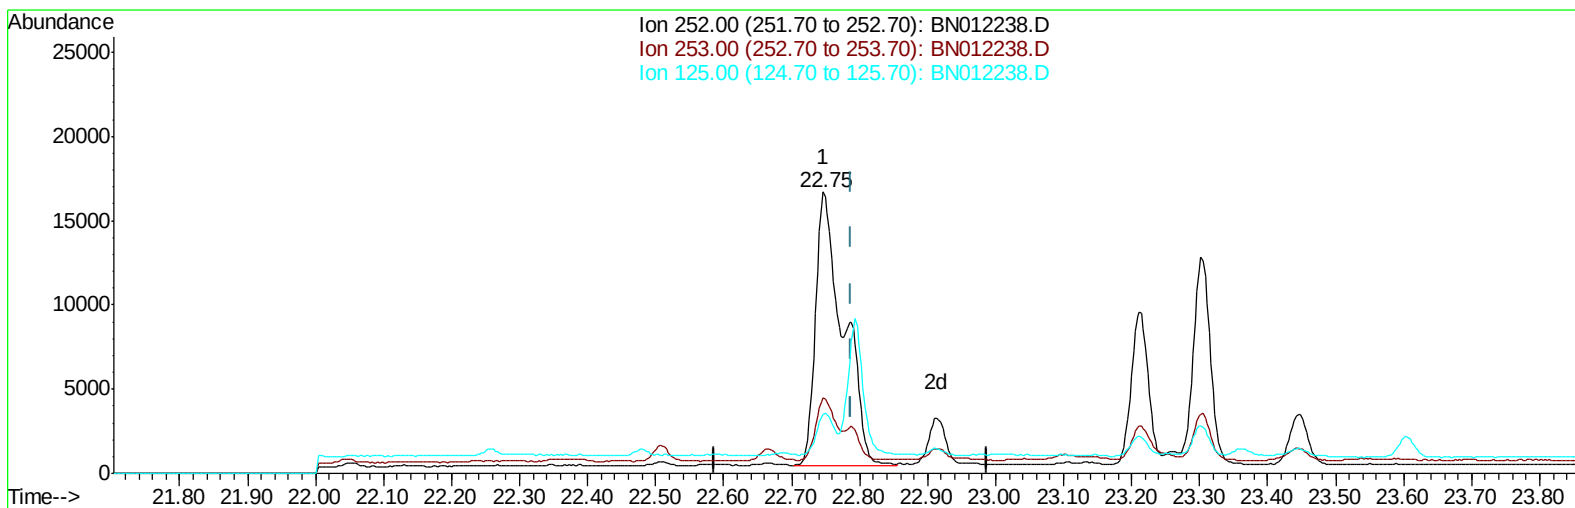

TIC: BN012238.D

(22) Benzo(k)fluoranthene

22.747min (-0.041) 1.34ng/ul

response 45824

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	26.90
125.00	16.10	21.14#
0.00	0.00	0.00