
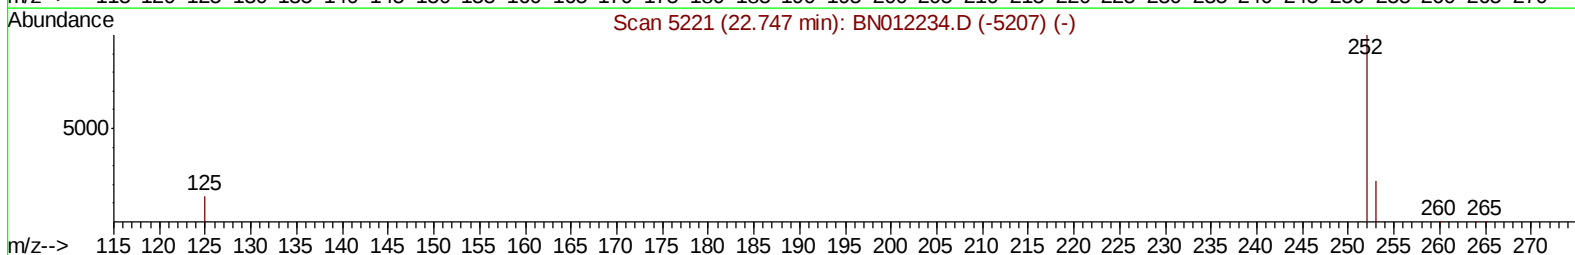
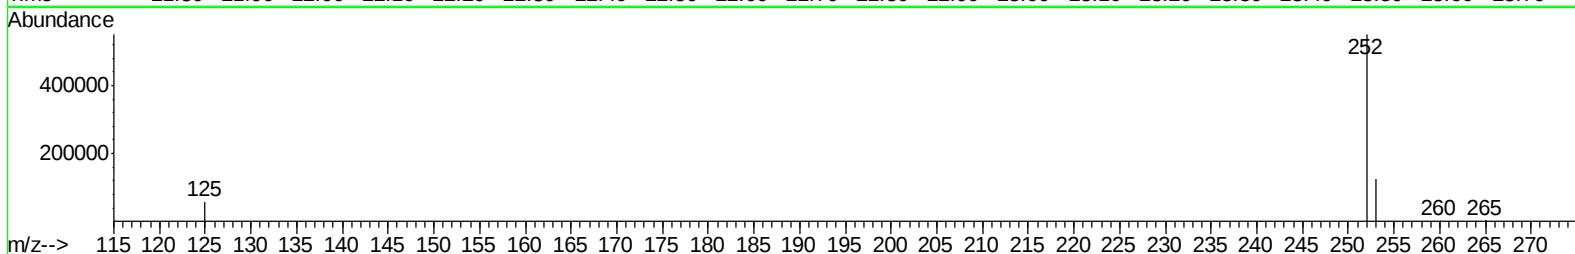


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012241.D
Acq On : 15 Oct 2020 21:01
Operator : CG/JU
Sample : L4235-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 16 01:27:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

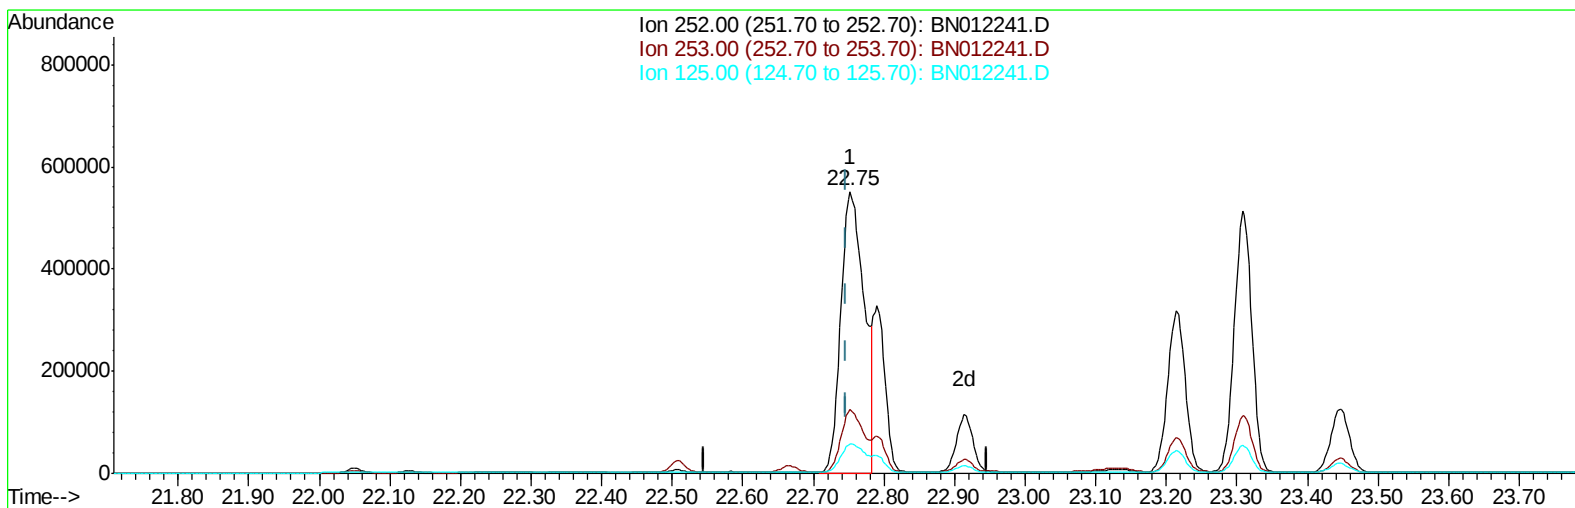

TIC: BN012241.D

(21) Benzo(b)fluoranthene

22.752min (+0.006) 31.99ng/ul m

response 1256112

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	22.62
125.00	18.40	10.48
0.00	0.00	0.00