
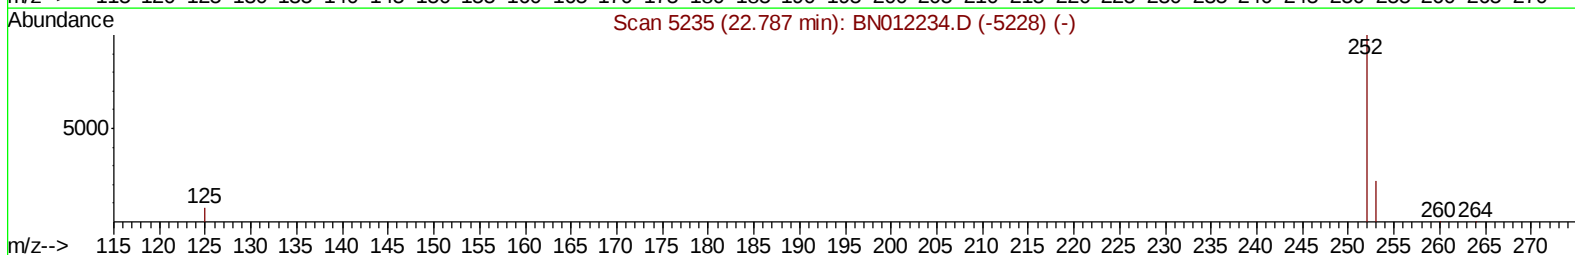
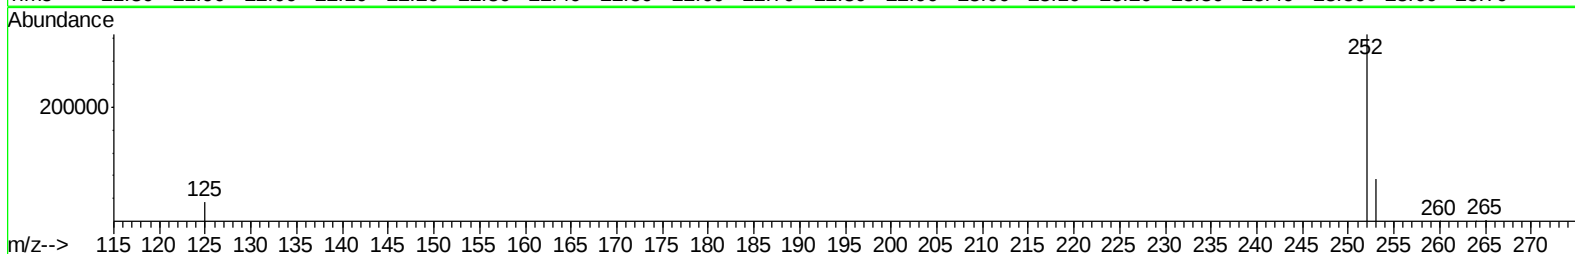


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012241.D
Acq On : 15 Oct 2020 21:01
Operator : CG/JU
Sample : L4235-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 16 01:27:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

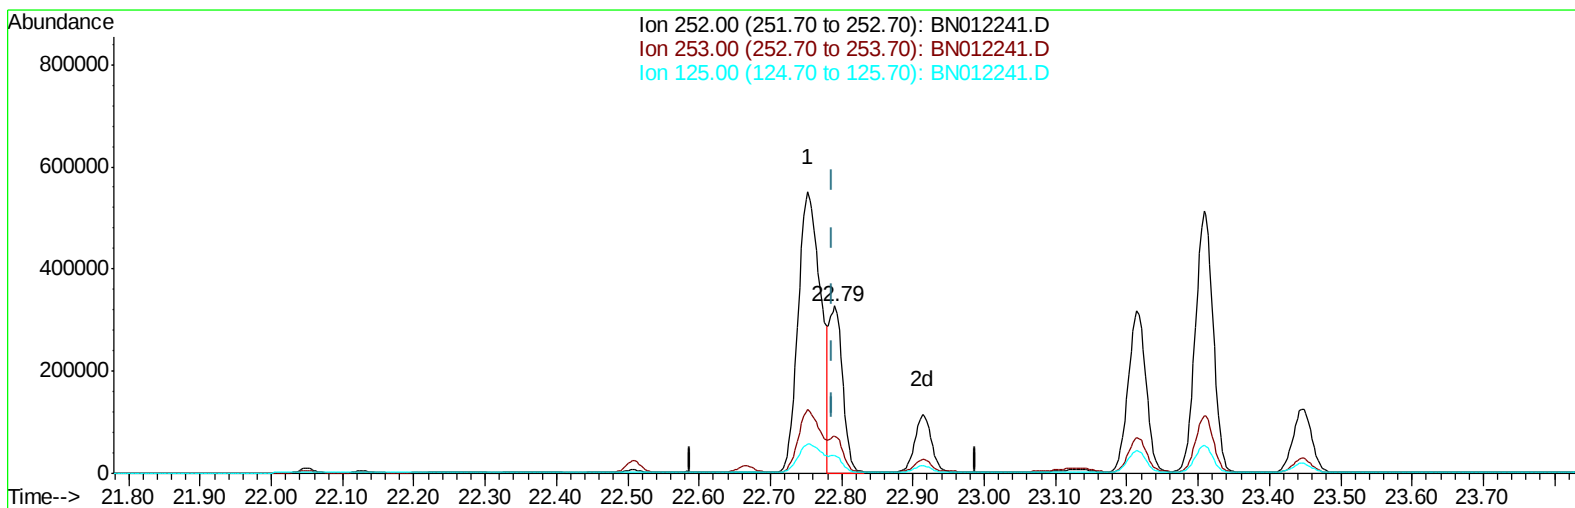

TIC: BN012241.D

(22) Benzo(k)fluoranthene

22.790min (+0.003) 10.22ng/ul m

response 444119

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	22.55#
125.00	16.10	10.72#
0.00	0.00	0.00