
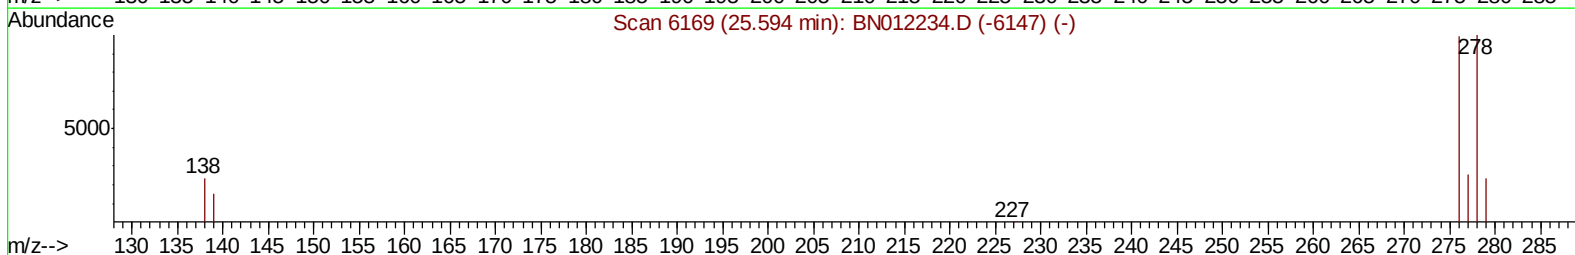
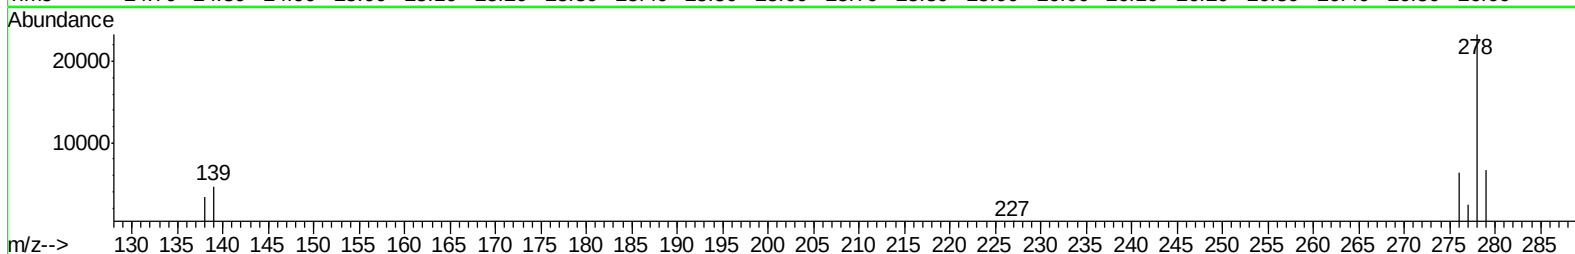


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012241.D
Acq On : 15 Oct 2020 21:01
Operator : CG/JU
Sample : L4235-06
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 16 01:27:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

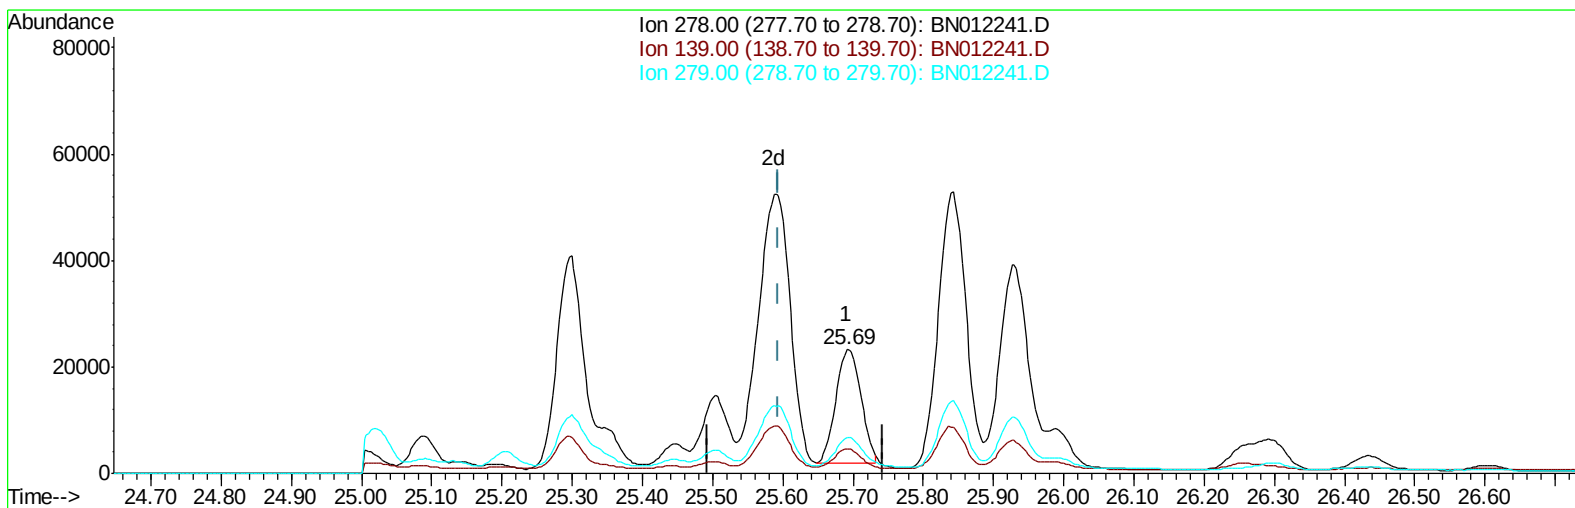

TIC: BN012241.D

(25) Dibenzo(a,h)anthracene

25.691min (+0.097) 1.35ng/ul

response 52856

Ion	Exp%	Act%
278.00	100	100
139.00	19.60	20.00
279.00	32.50	28.72
0.00	0.00	0.00