
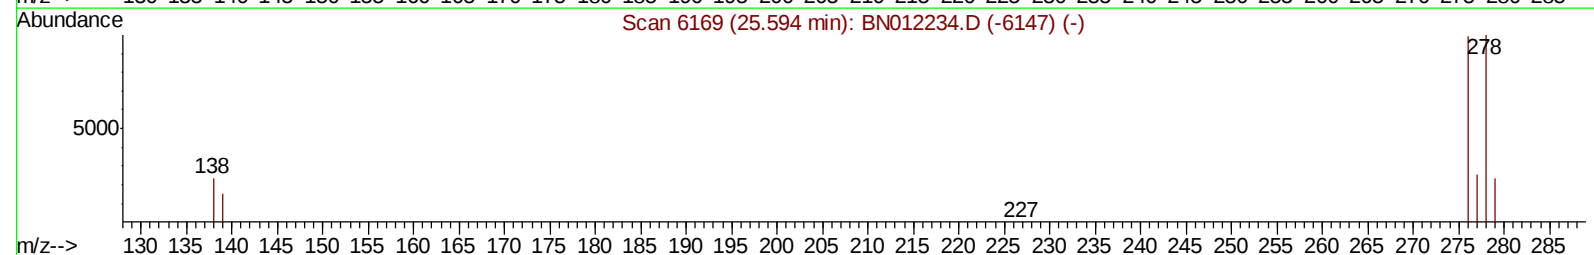
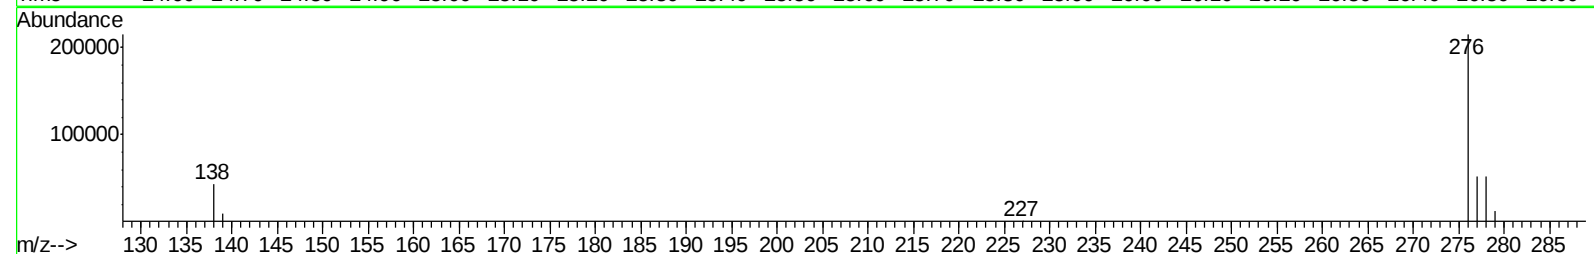


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012241.D
 Acq On : 15 Oct 2020 21:01
 Operator : CG/JU
 Sample : L4235-06
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Quant Time: Oct 16 01:27:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:19:50 2020
 Response via : Initial Calibration

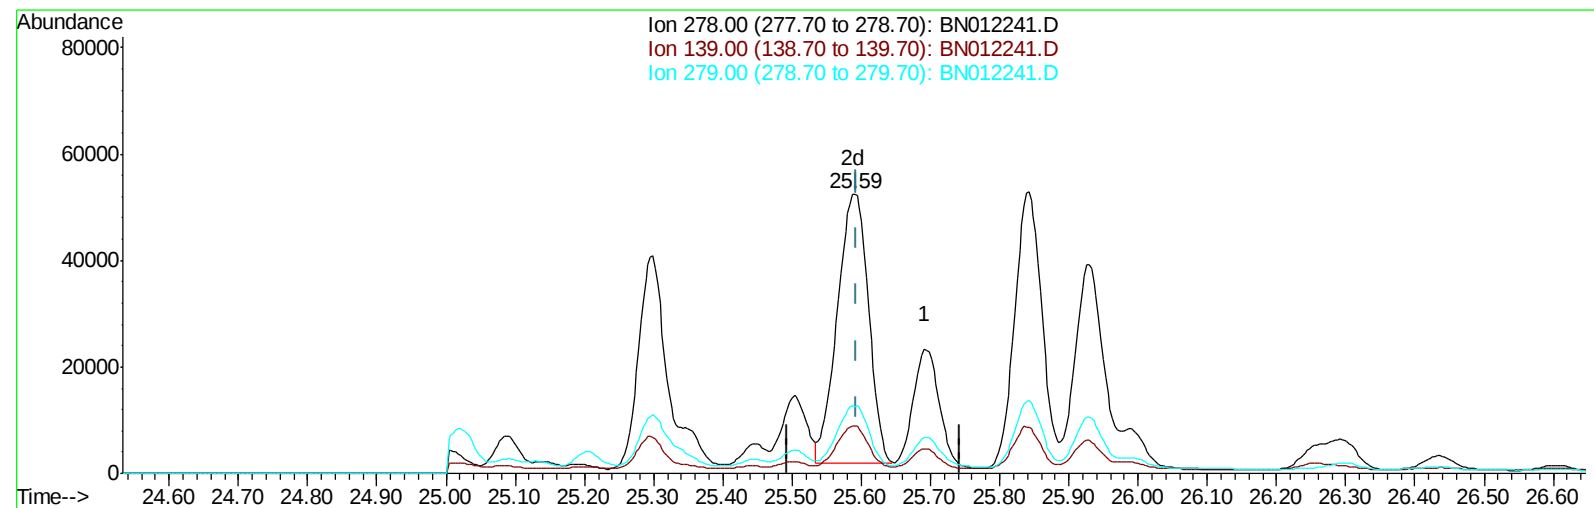

TIC: BN012241.D

(25) Dibenzo(a,h)anthracene

25.587min (-0.007) 4.01ng/ul m

response 157521

Ion	Exp%	Act%
278.00	100	100
139.00	19.60	17.10
279.00	32.50	24.13#
0.00	0.00	0.00