
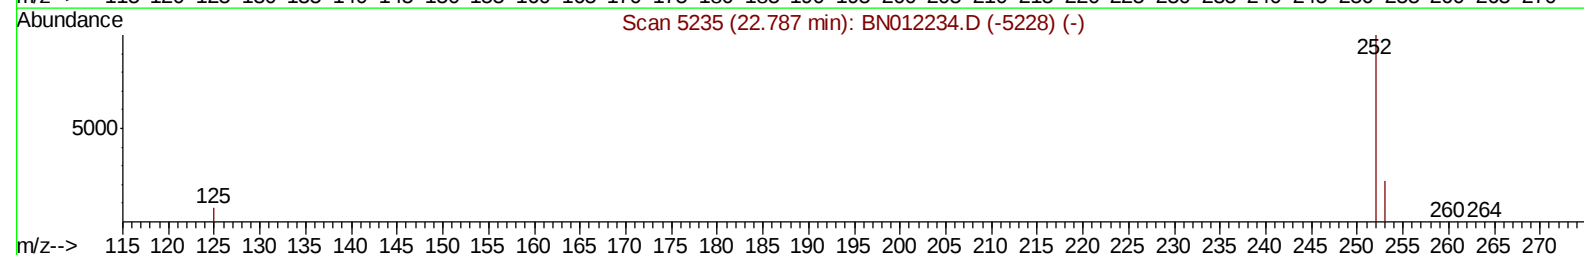
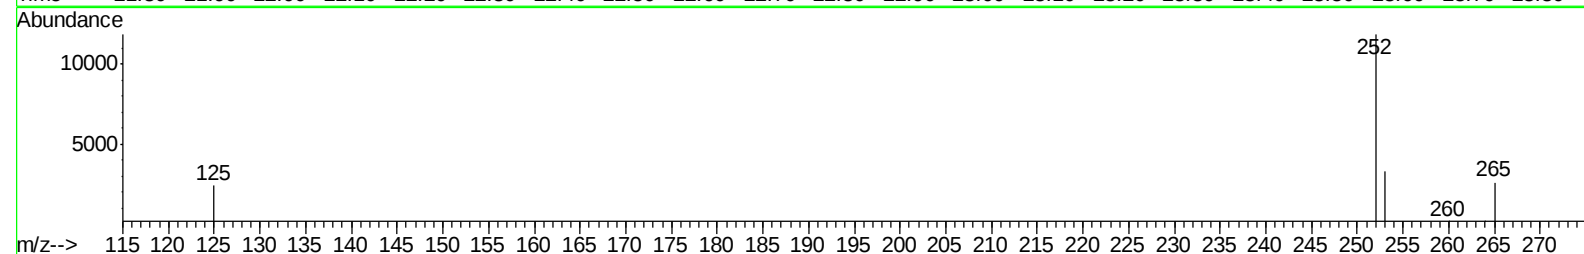


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012242.D
Acq On : 15 Oct 2020 21:37
Operator : CG/JU
Sample : L4235-09
Misc :
ALS Vial : 54 Sample Multiplier: 1

Quant Time: Oct 16 01:27:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

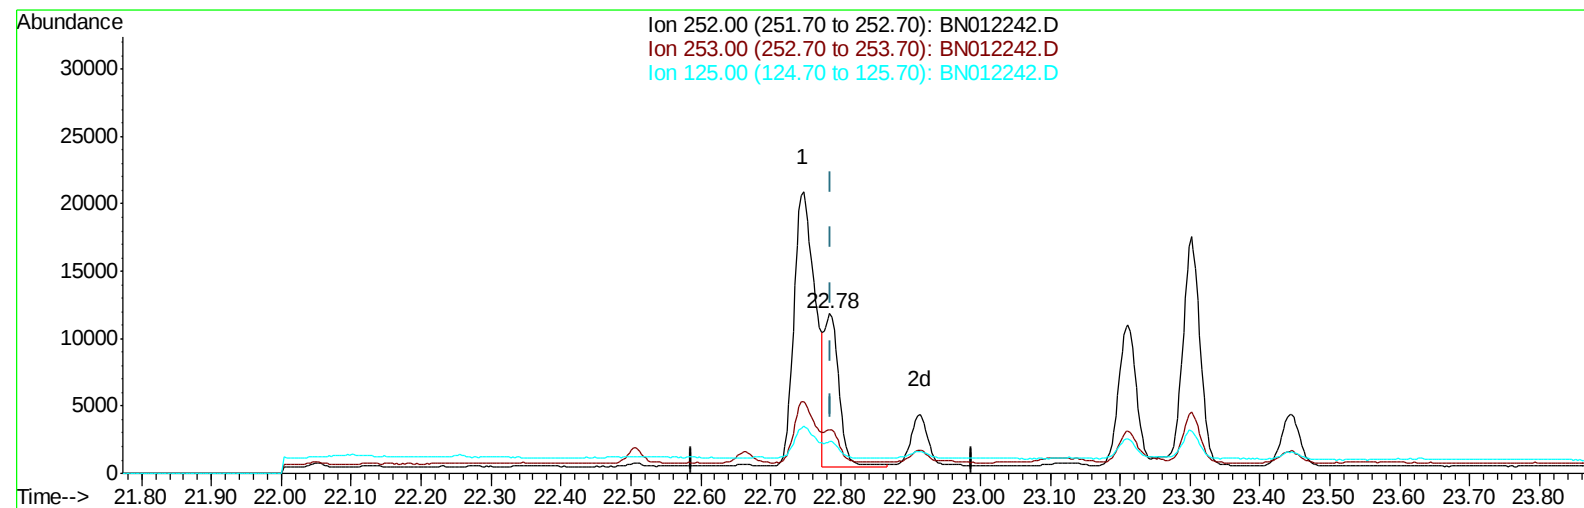

TIC: BN012242.D

(22) Benzo(k)fluoranthene

22.785min (-0.003) 0.50ng/ul m

response 17068

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.54
125.00	16.10	20.04#
0.00	0.00	0.00