
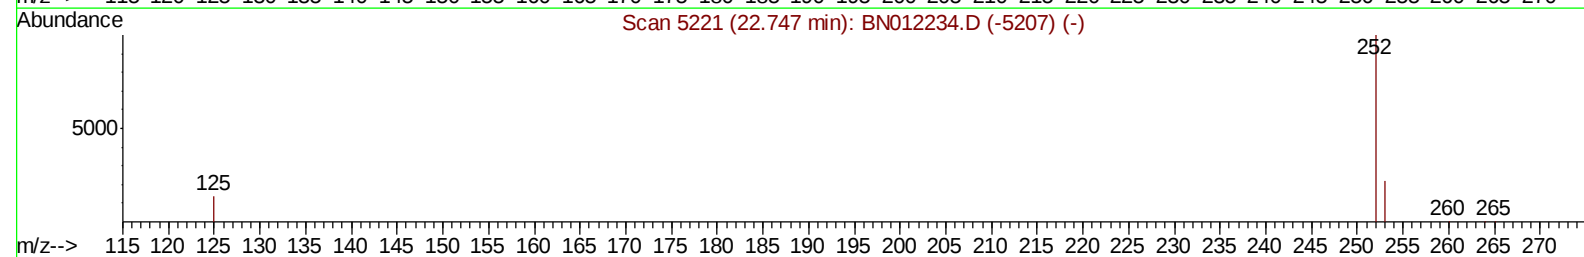
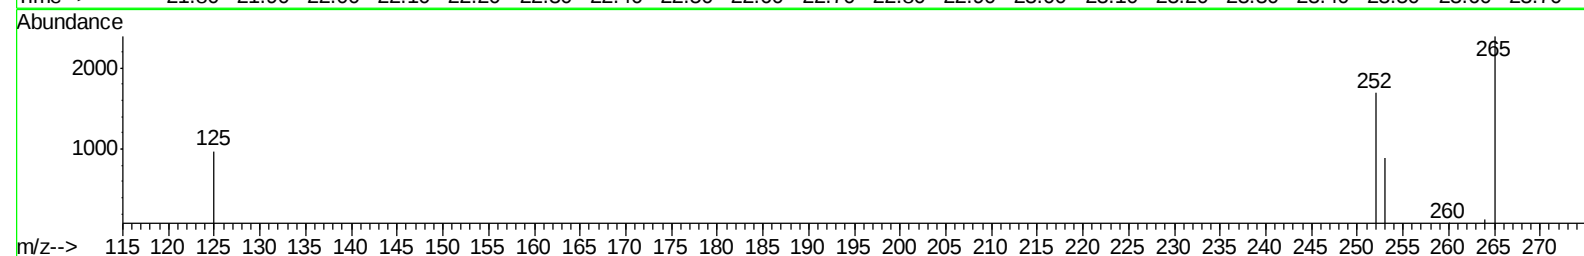


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012246.D
 Acq On : 16 Oct 2020 00:02
 Operator : CG/JU
 Sample : L4235-14
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Quant Time: Oct 16 02:18:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:19:50 2020
 Response via : Initial Calibration

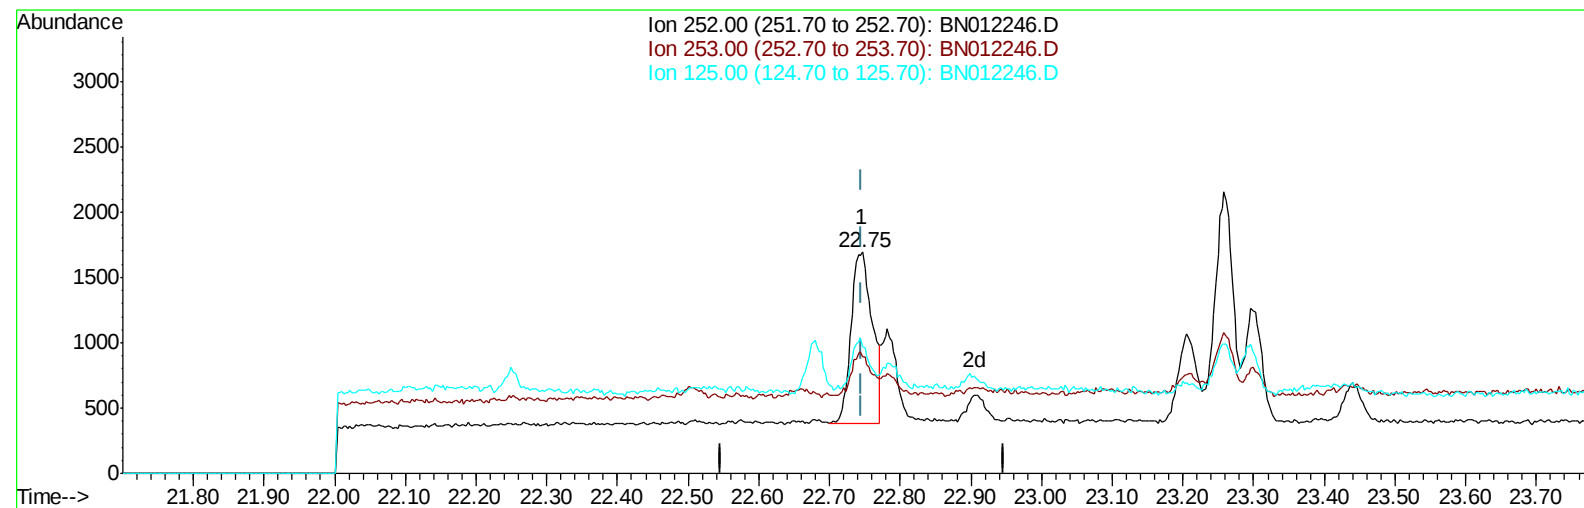

TIC: BN012246.D

(21) Benzo(b)fluoranthene

22.747min (+0.000) 0.07ng/ul m

response 2694

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	52.93
125.00	18.40	57.60#
0.00	0.00	0.00