
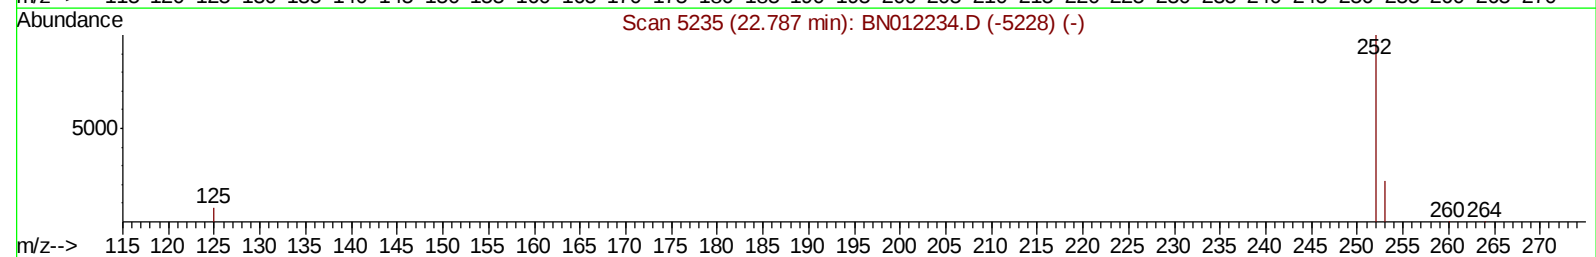
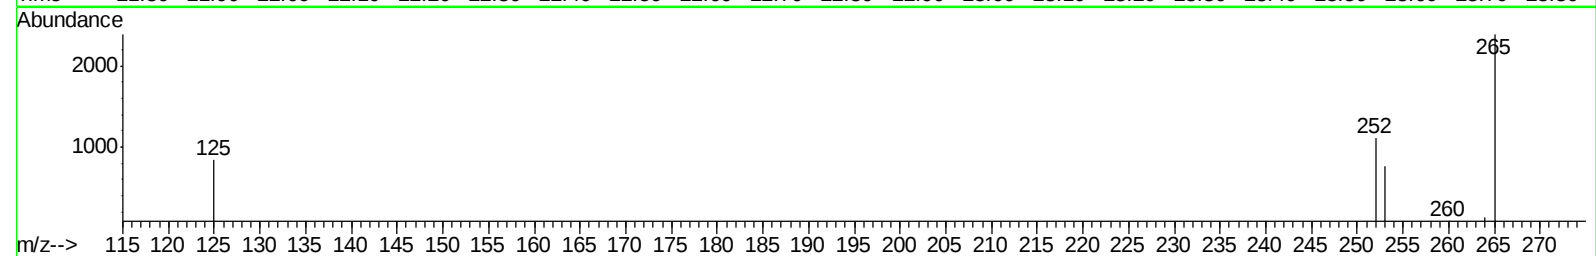


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012246.D
Acq On : 16 Oct 2020 00:02
Operator : CG/JU
Sample : L4235-14
Misc :
ALS Vial : 58 Sample Multiplier: 1

Quant Time: Oct 16 02:18:41 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

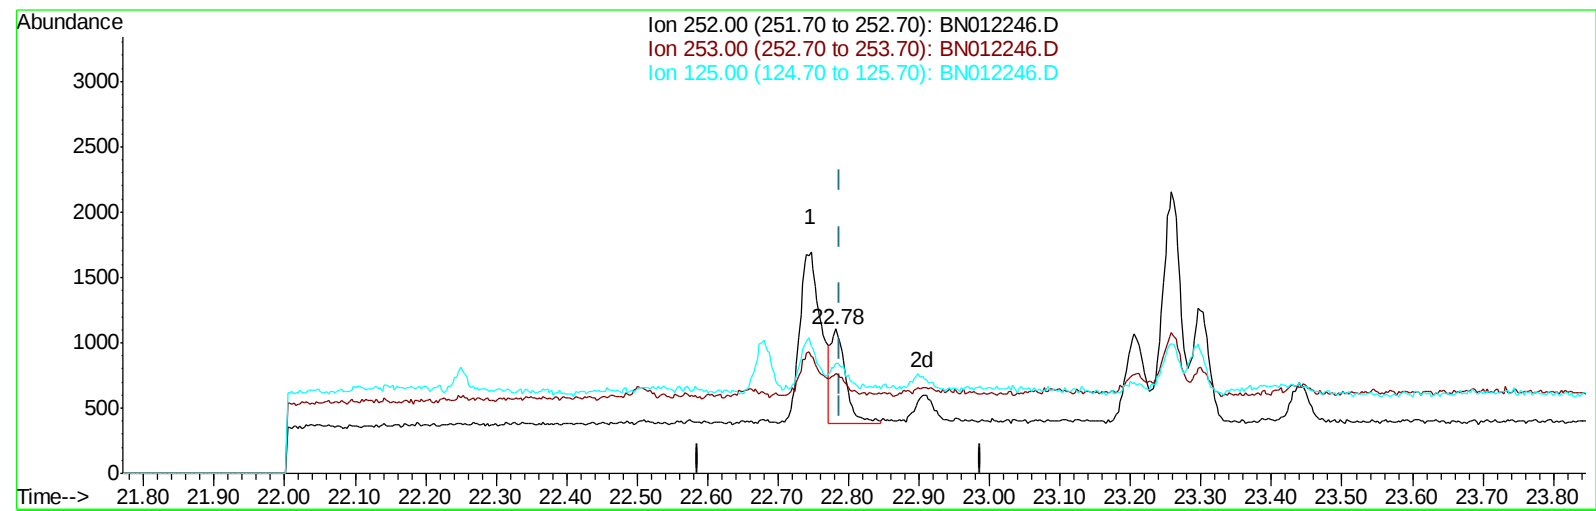

TIC: BN012246.D

(22) Benzo(k)fluoranthene

22.782min (-0.006) 0.03ng/ul m

response 1094

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	69.38#
125.00	16.10	76.00#
0.00	0.00	0.00