
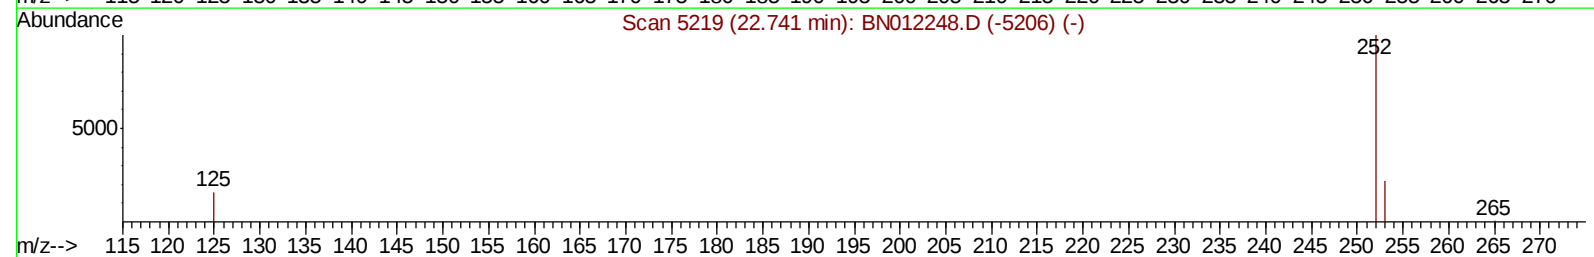
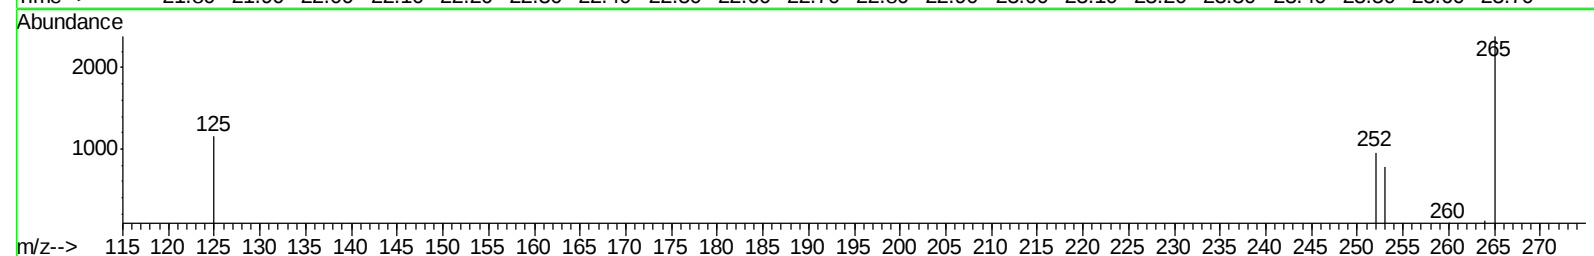


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012250.D
 Acq On : 16 Oct 2020 03:02
 Operator : CG/JU
 Sample : L4235-12
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Quant Time: Oct 16 06:37:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 06:21:01 2020
 Response via : Initial Calibration

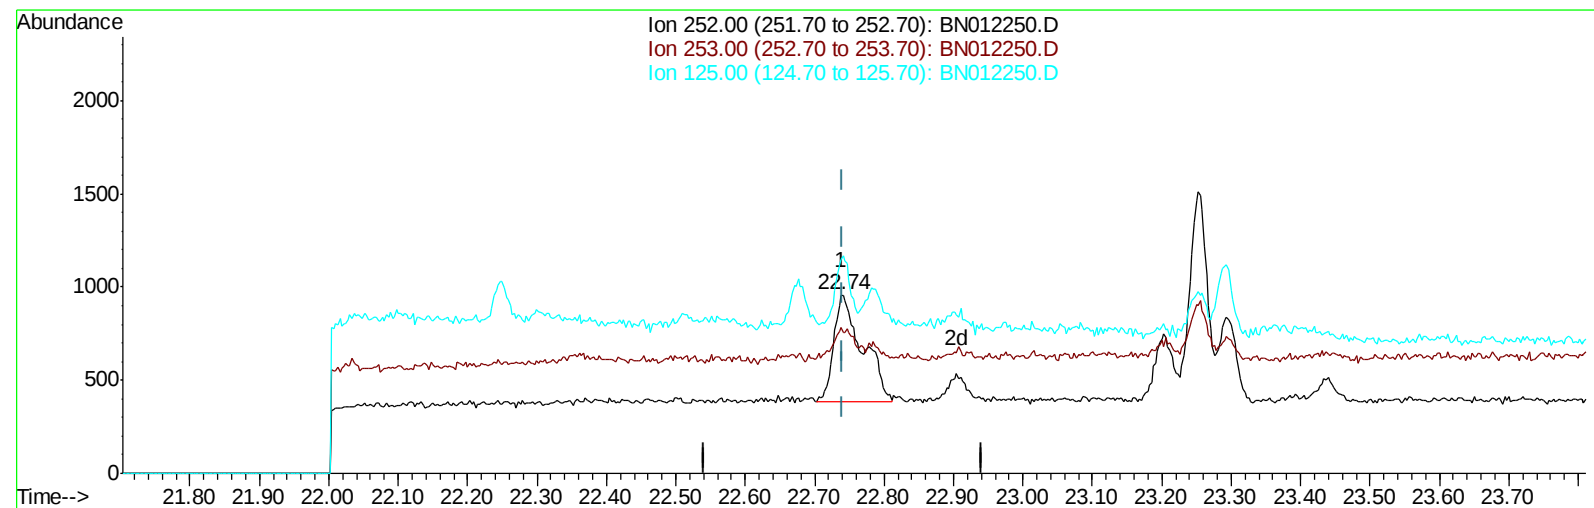

TIC: BN012250.D

(21) Benzo(b)fluoranthene
 22.738min (-0.003) 0.04ng/ul
 response 1676

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	81.78#
125.00	18.40	120.31#
0.00	0.00	0.00