
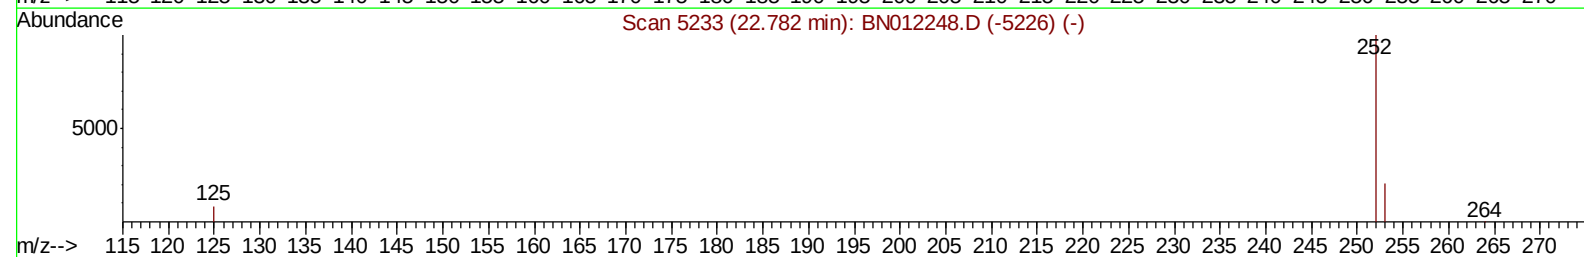
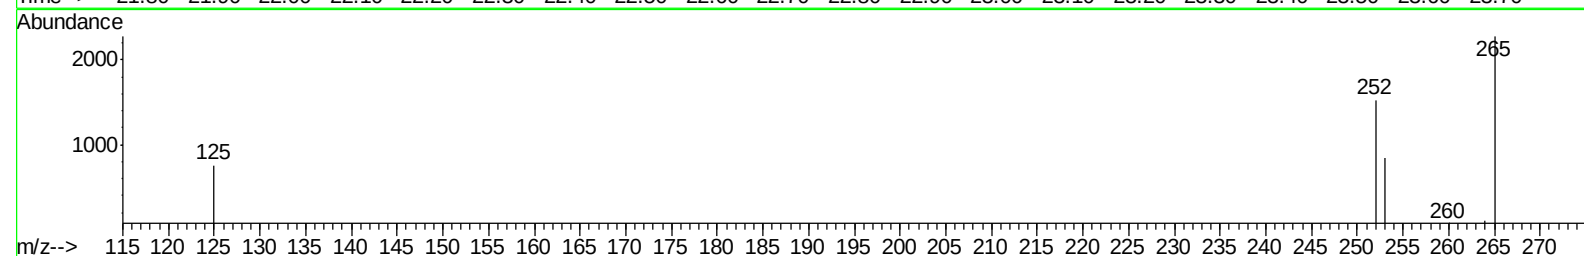


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012251.D
Acq On : 16 Oct 2020 03:38
Operator : CG/JU
Sample : L4235-18
Misc :
ALS Vial : 63 Sample Multiplier: 1

Quant Time: Oct 16 06:28:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 06:21:01 2020
Response via : Initial Calibration

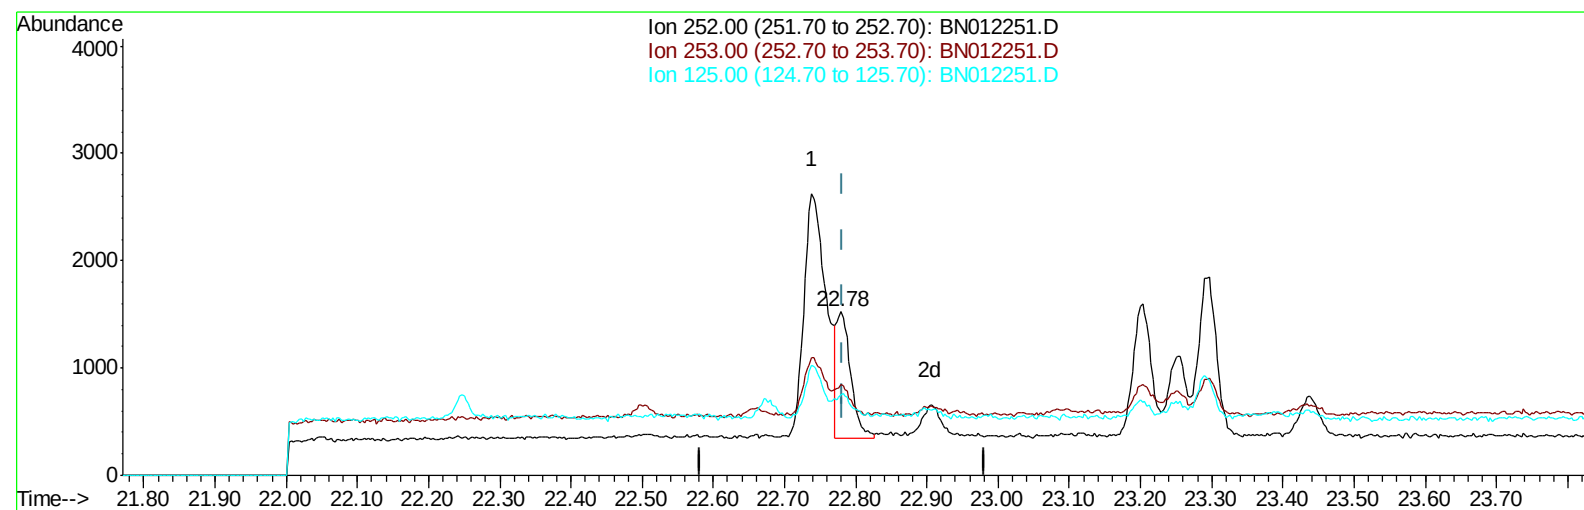

TIC: BN012251.D

(22) Benzo(k)fluoranthene

22.779min (-0.003) 0.04ng/ul m

response 1628

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	55.55#
125.00	16.10	49.64#
0.00	0.00	0.00