
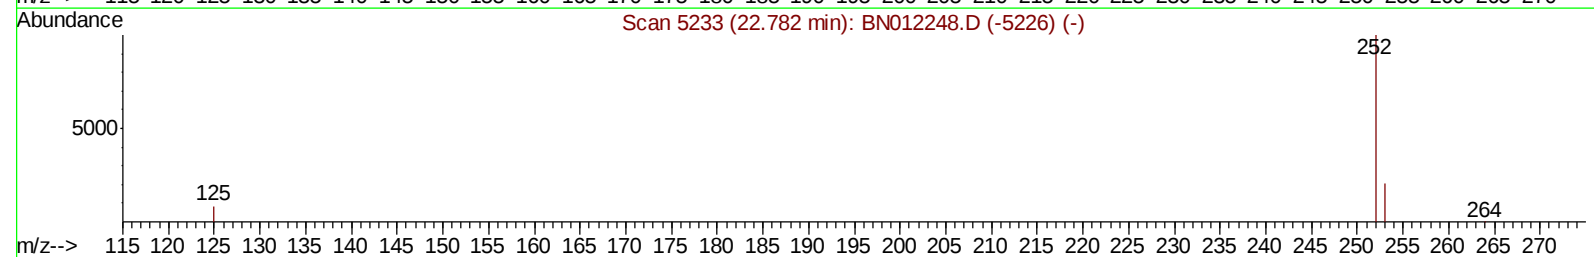
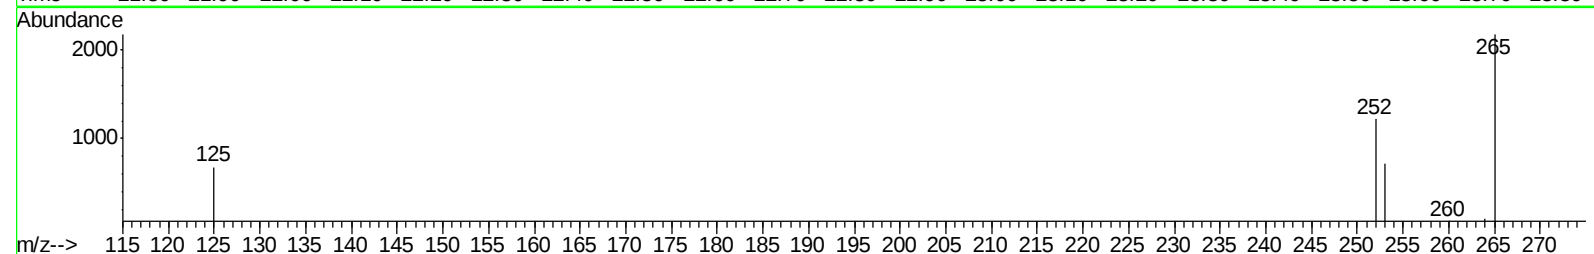


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012255.D
Acq On : 16 Oct 2020 06:03
Operator : CG/JU
Sample : L4235-19
Misc :
ALS Vial : 67 Sample Multiplier: 1

Quant Time: Oct 16 06:48:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 06:21:01 2020
Response via : Initial Calibration

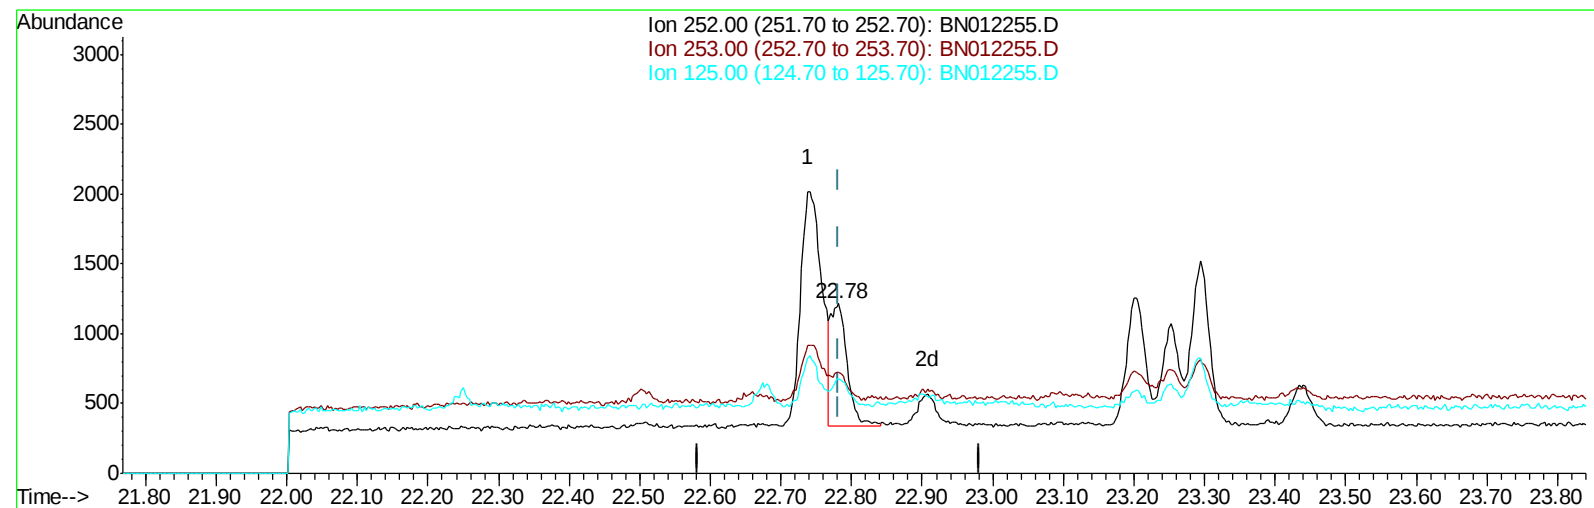

TIC: BN012255.D

(22) Benzo(k)fluoranthene

22.782min (+0.000) 0.04ng/ul m

response 1406

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	59.28#
125.00	16.10	55.91#
0.00	0.00	0.00