
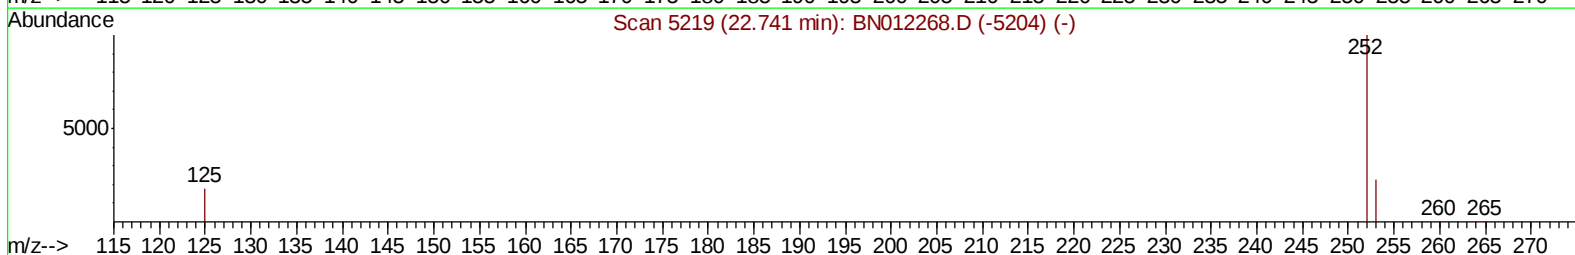
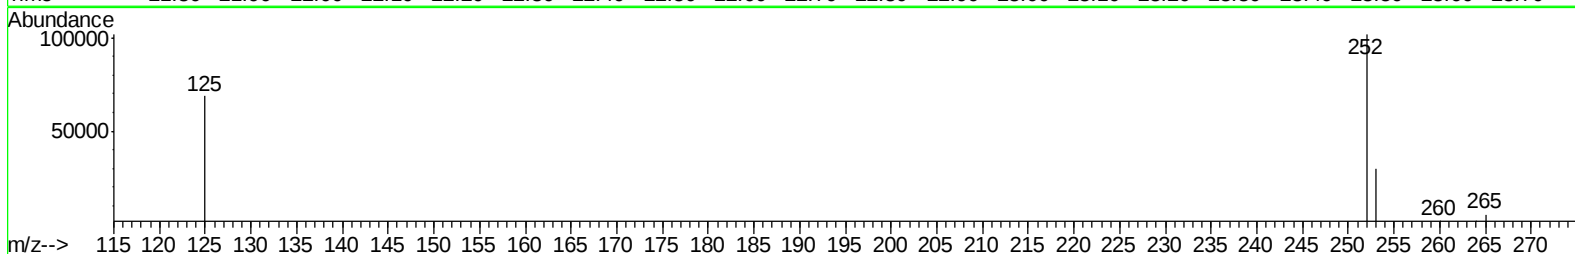


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012273.D
Acq On : 16 Oct 2020 18:50
Operator : CG/JU
Sample : L4201-11
Misc :
ALS Vial : 85 Sample Multiplier: 1

Quant Time: Oct 17 02:33:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 17 02:30:59 2020
Response via : Initial Calibration

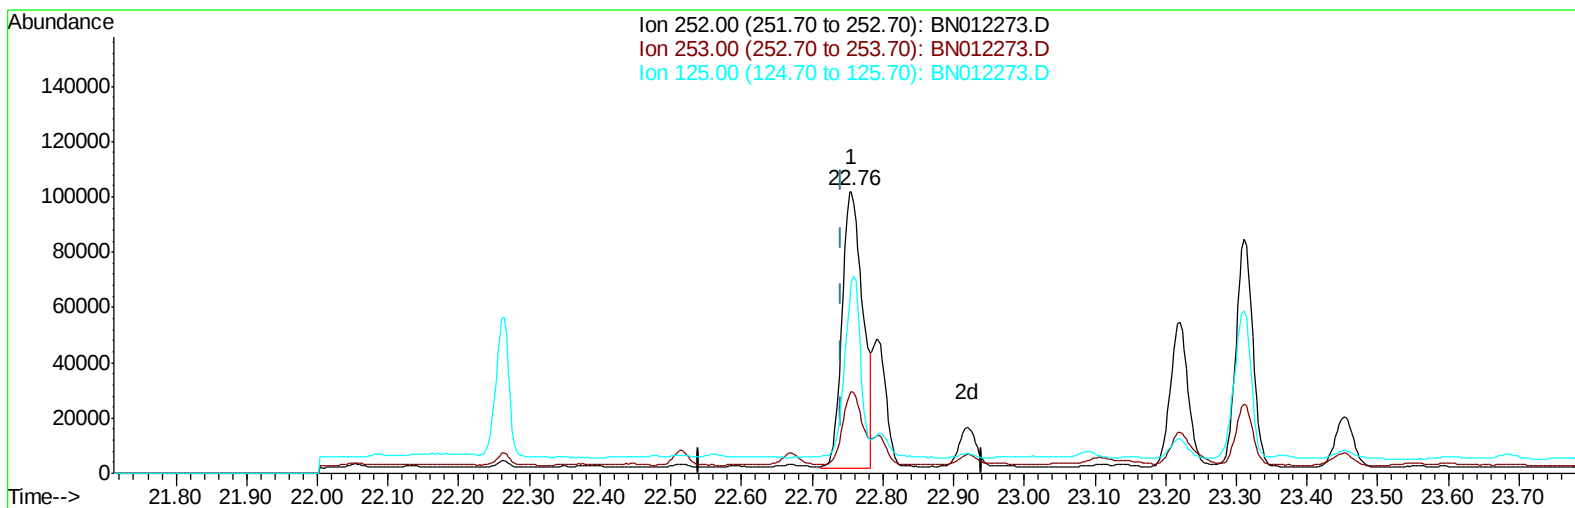

TIC: BN012273.D

(21) Benzo(b)fluoranthene

22.756min (+0.015) 6.70ng/ul m

response 201613

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	29.10
125.00	18.40	67.58#
0.00	0.00	0.00