
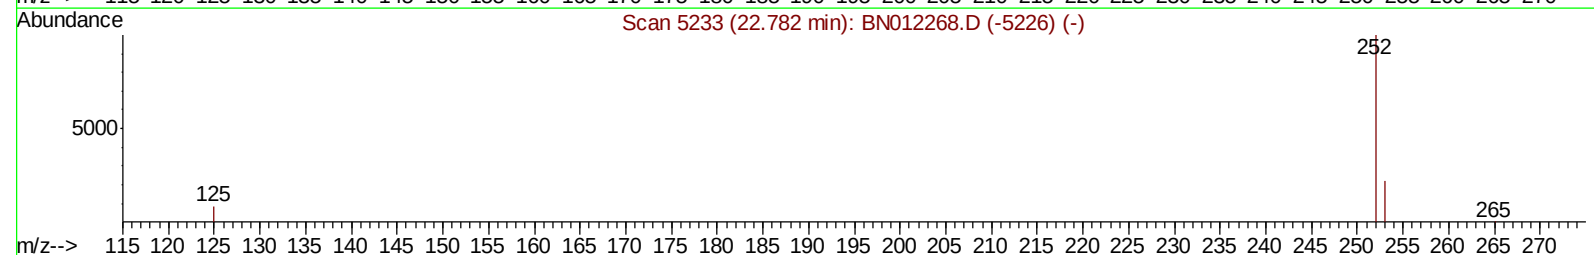
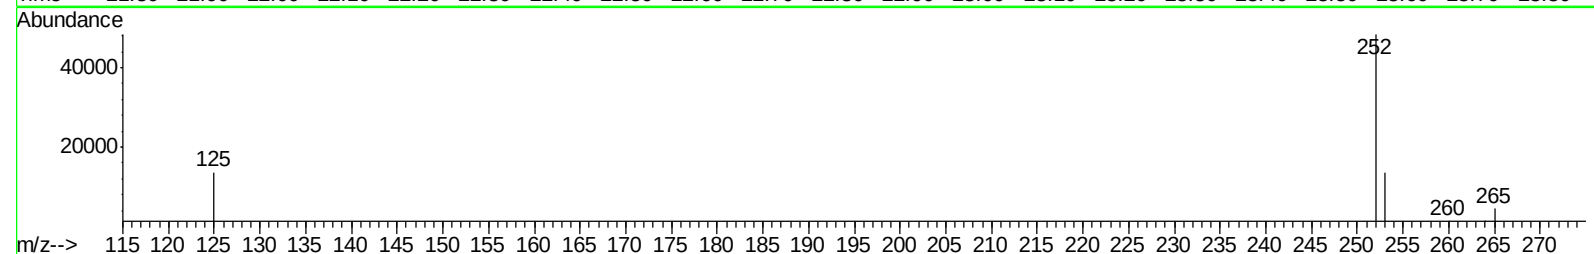


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012273.D
 Acq On : 16 Oct 2020 18:50
 Operator : CG/JU
 Sample : L4201-11
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Quant Time: Oct 17 02:33:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 17 02:30:59 2020
 Response via : Initial Calibration

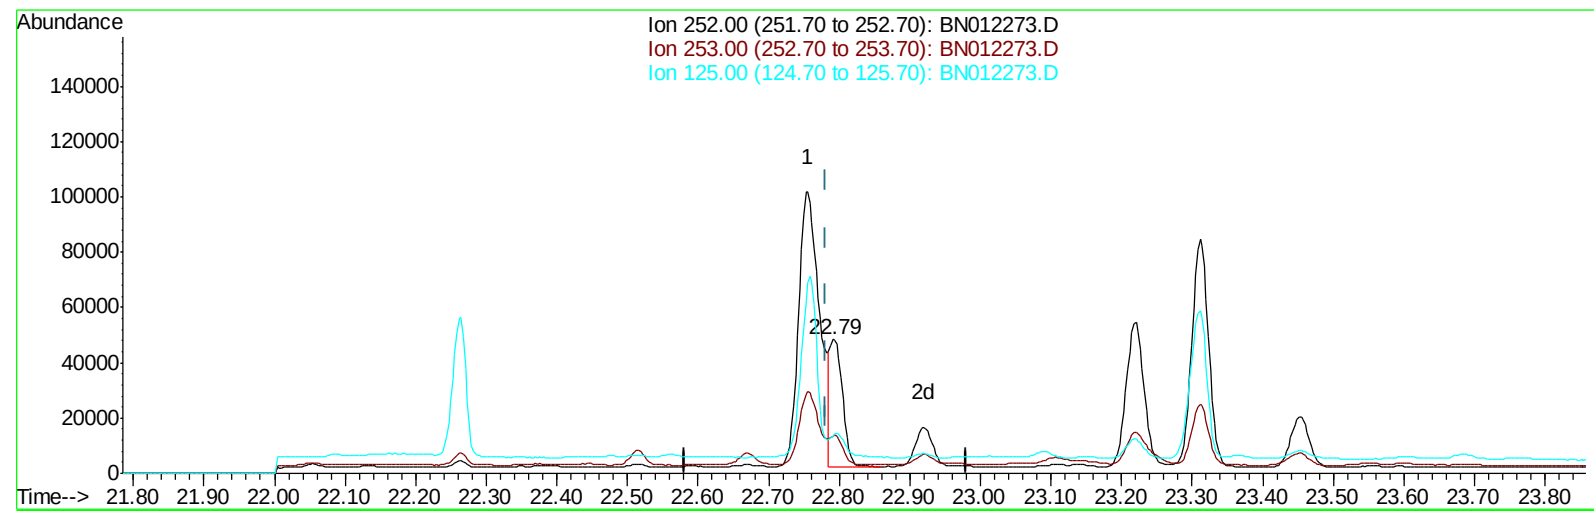

TIC: BN012273.D

(22) Benzo(k)fluoranthene

22.791min (+0.009) 1.69ng/ul m

response 56174

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.86
125.00	16.10	28.12#
0.00	0.00	0.00