
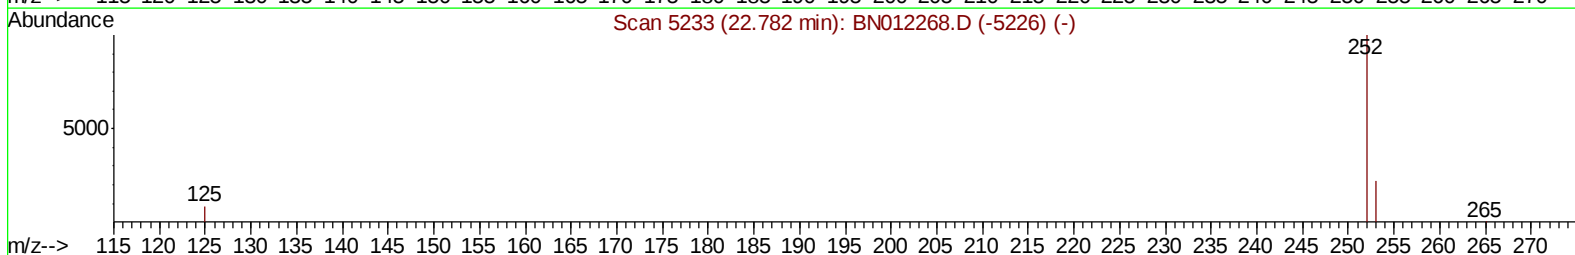
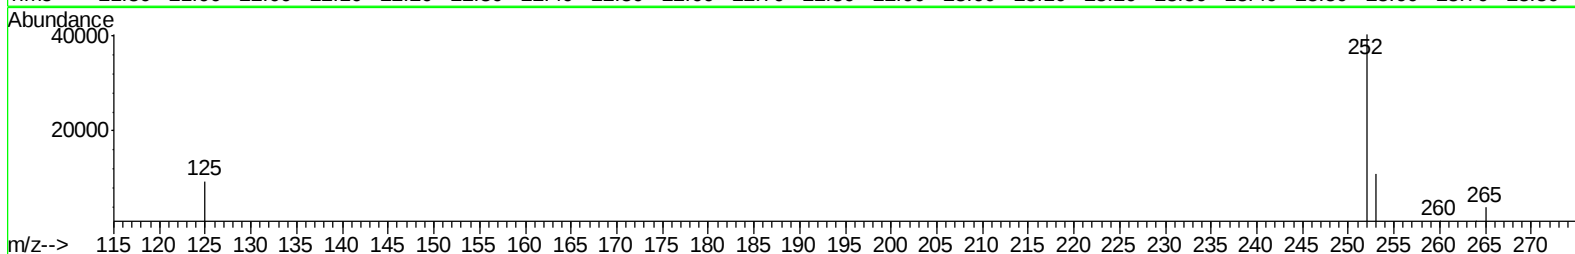


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012274.D
Acq On : 16 Oct 2020 19:27
Operator : CG/JU
Sample : L4201-17
Misc :
ALS Vial : 86 Sample Multiplier: 1

Quant Time: Oct 17 02:33:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 17 02:30:59 2020
Response via : Initial Calibration

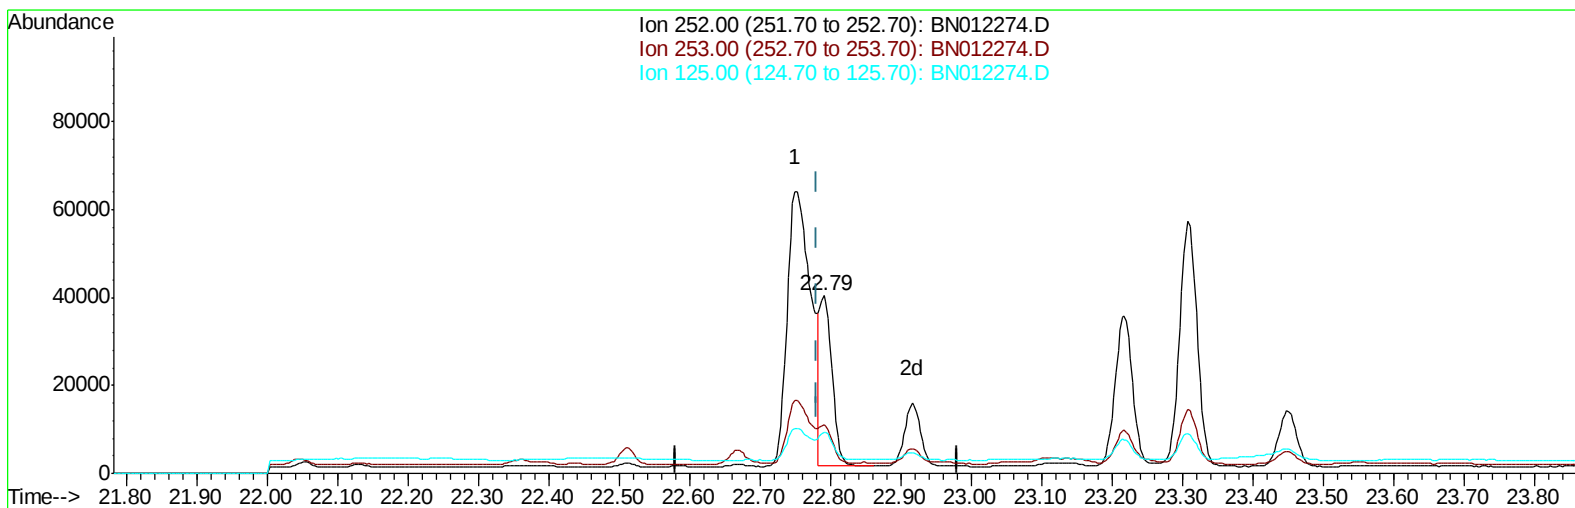

TIC: BN012274.D

(22) Benzo(k)fluoranthene

22.790min (+0.009) 1.60ng/ul m

response 48382

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.10
125.00	16.10	23.22#
0.00	0.00	0.00