
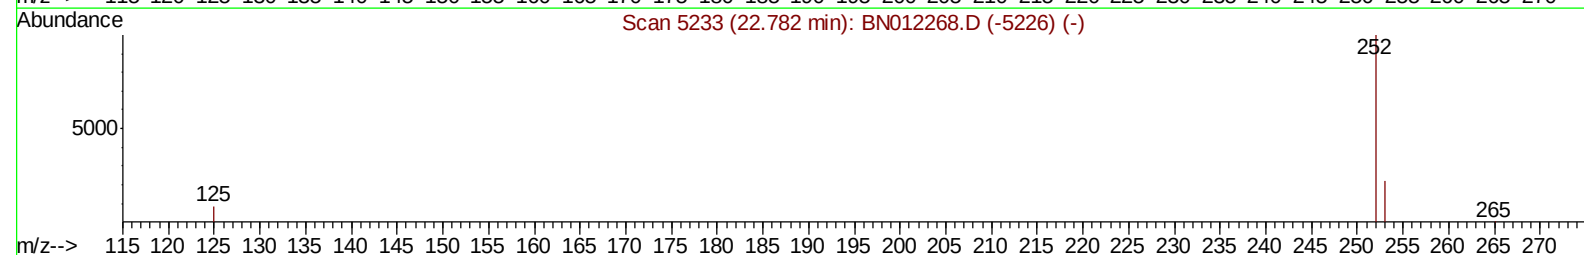
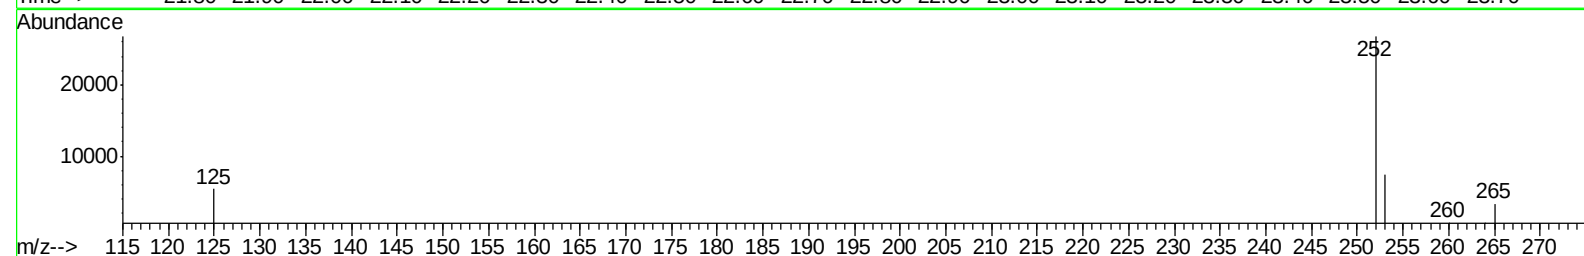


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012275.D
 Acq On : 16 Oct 2020 20:03
 Operator : CG/JU
 Sample : L4201-03DL 5X
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Quant Time: Oct 17 02:34:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 17 02:30:59 2020
 Response via : Initial Calibration

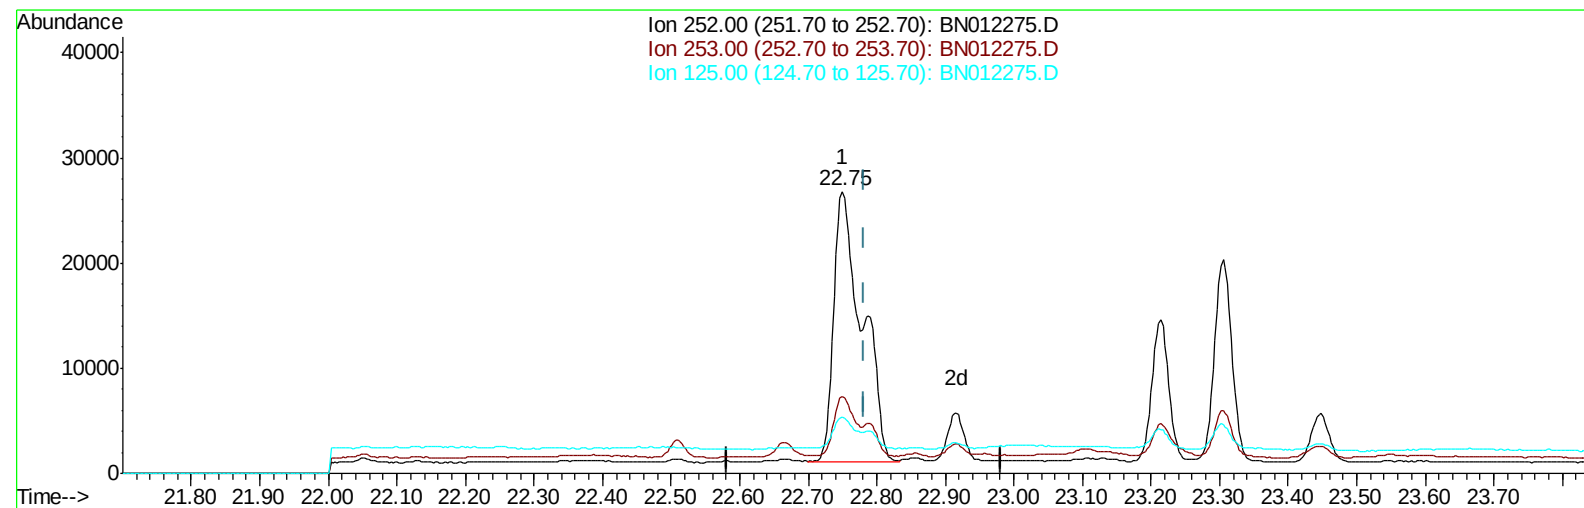

TIC: BN012275.D

(22) Benzo(k)fluoranthene

22.750min (-0.032) 2.56ng/ul

response 73363

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	27.49
125.00	16.10	20.04#
0.00	0.00	0.00