
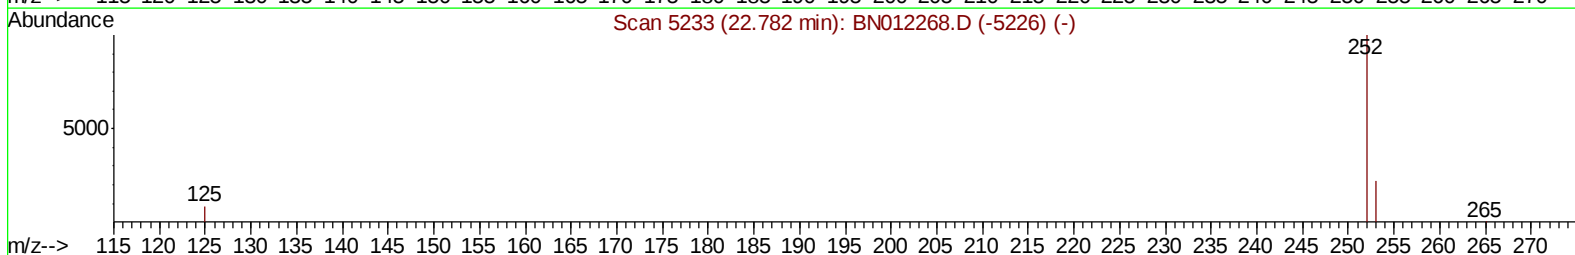
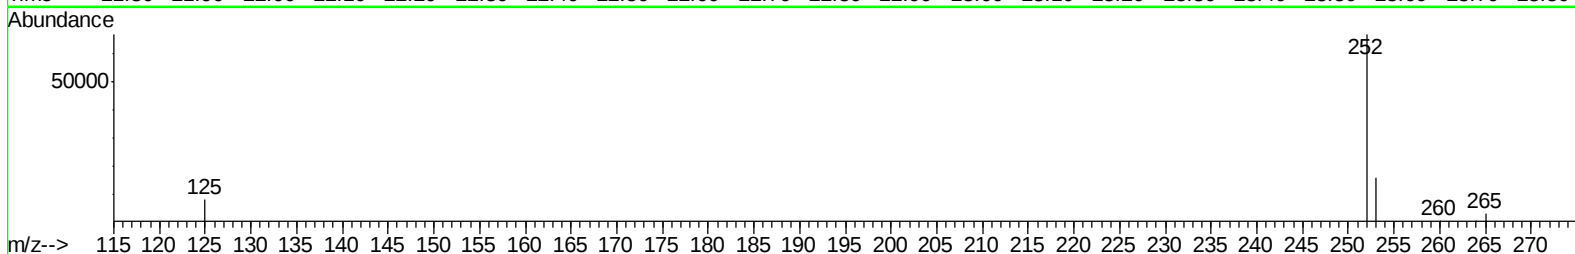


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012276.D
Acq On : 16 Oct 2020 20:40
Operator : CG/JU
Sample : L4201-18DL 5X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Quant Time: Oct 16 23:50:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 23:42:05 2020
Response via : Initial Calibration

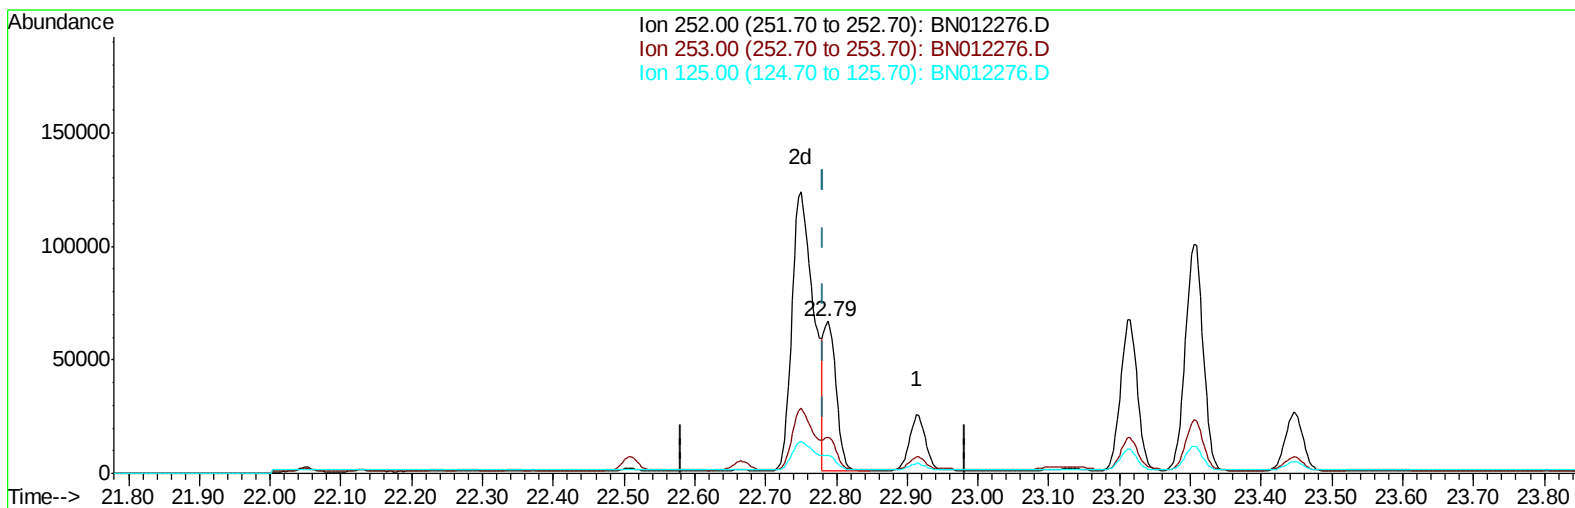

TIC: BN012276.D

(22) Benzo(k)fluoranthene

22.788min (+0.006) 2.79ng/ul m

response 83410

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	23.92#
125.00	16.10	12.01#
0.00	0.00	0.00