
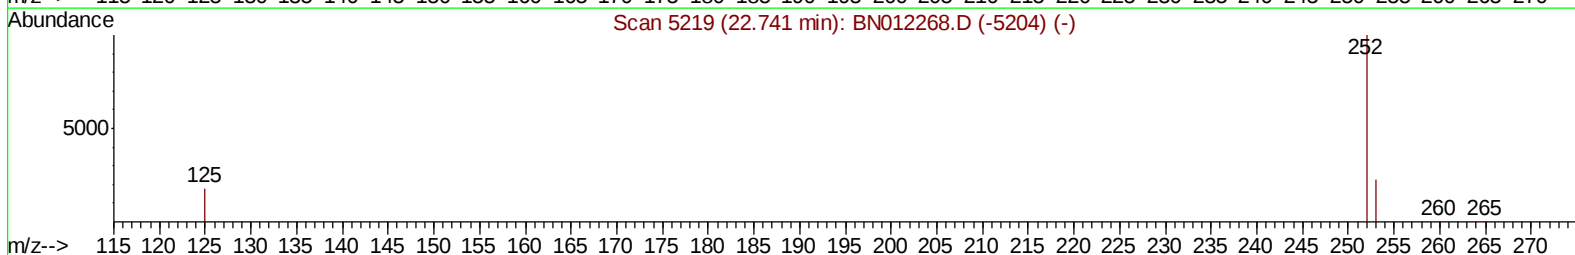
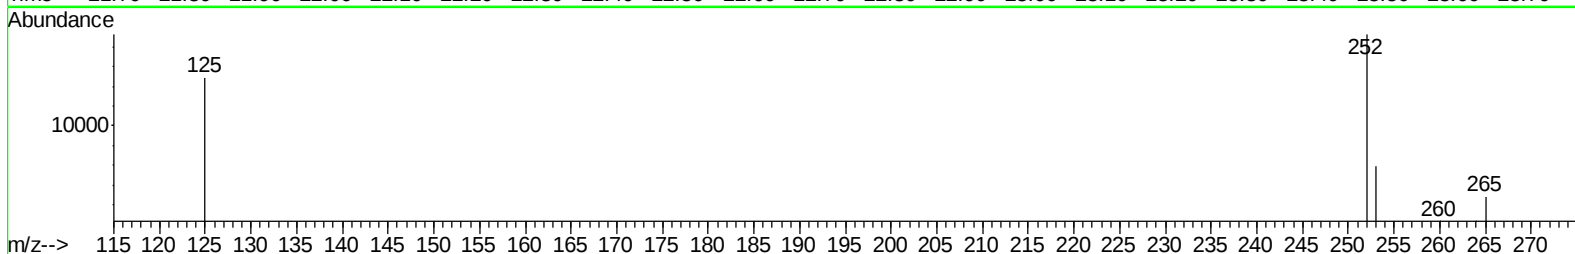


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012280.D
Acq On : 16 Oct 2020 23:05
Operator : CG/JU
Sample : L4201-11DL 5X
Misc :
ALS Vial : 92 Sample Multiplier: 1

Quant Time: Oct 16 23:50:45 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 23:42:05 2020
Response via : Initial Calibration

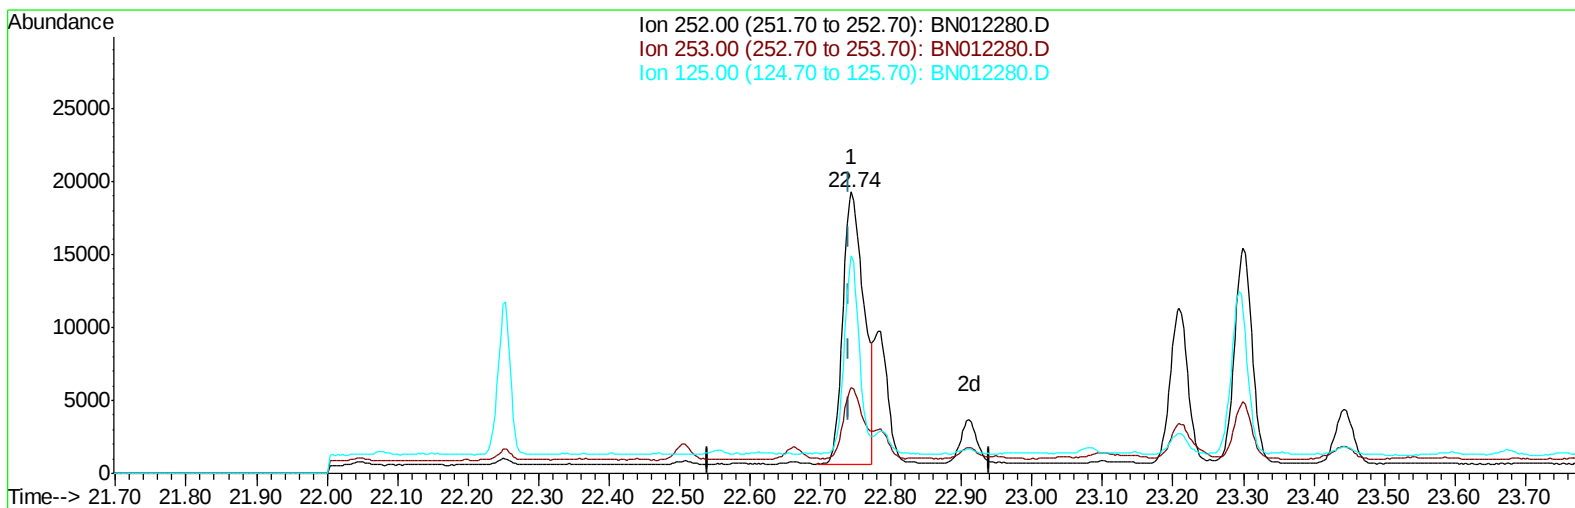

TIC: BN012280.D

(21) Benzo(b)fluoranthene

22.744min (+0.003) 1.21ng/ul m

response 39098

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	30.52
125.00	18.40	77.36#
0.00	0.00	0.00