
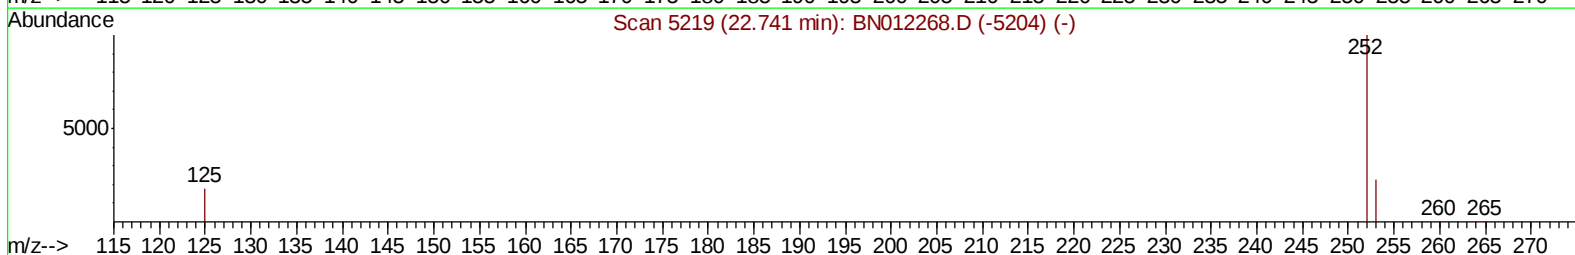
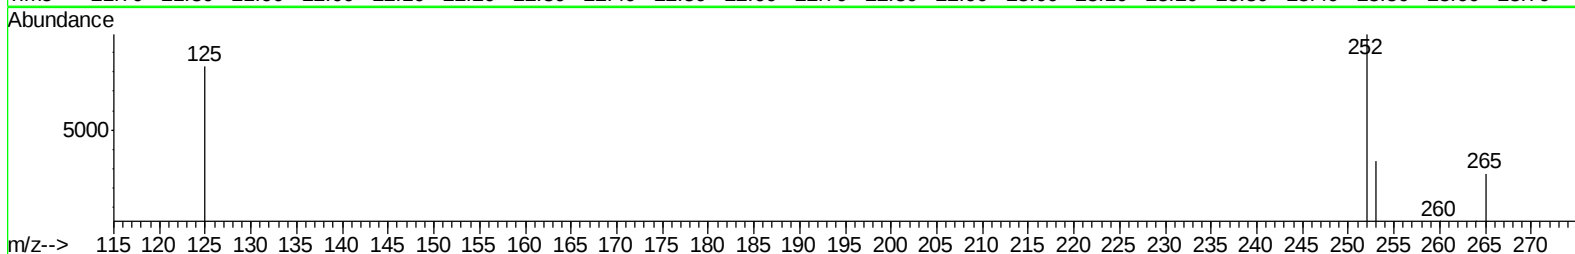


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012281.D
Acq On : 16 Oct 2020 23:41
Operator : CG/JU
Sample : L4201-11DL 10X
Misc :
ALS Vial : 93 Sample Multiplier: 1

Quant Time: Oct 17 00:28:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 23:42:05 2020
Response via : Initial Calibration

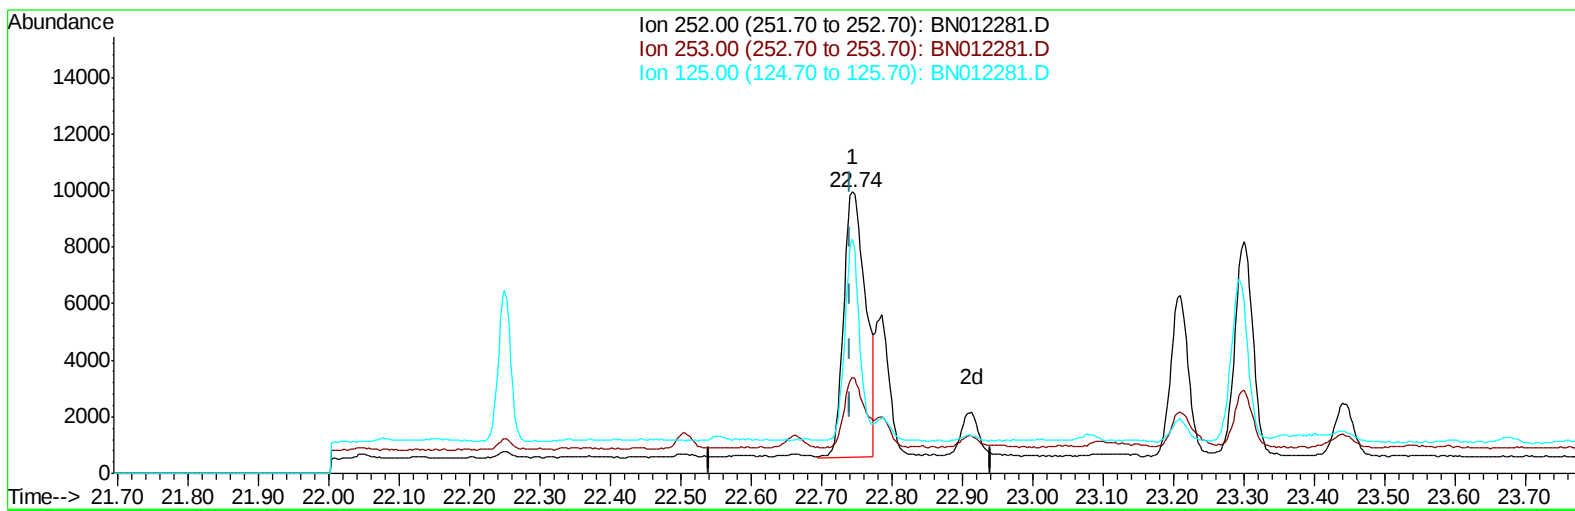

TIC: BN012281.D

(21) Benzo(b)fluoranthene

22.744min (+0.003) 0.65ng/ul m

response 20292

Ion	Exp%	Act%
252.00	100	100
253.00	30.80	34.14
125.00	18.40	83.18#
0.00	0.00	0.00