
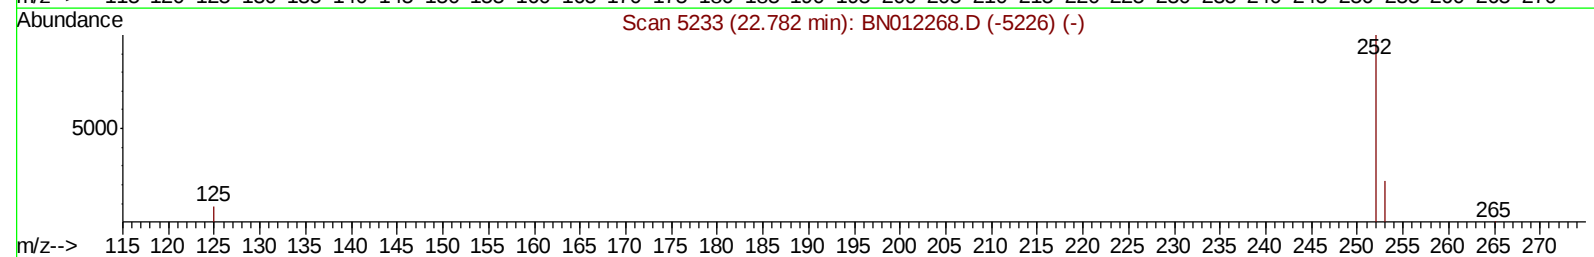
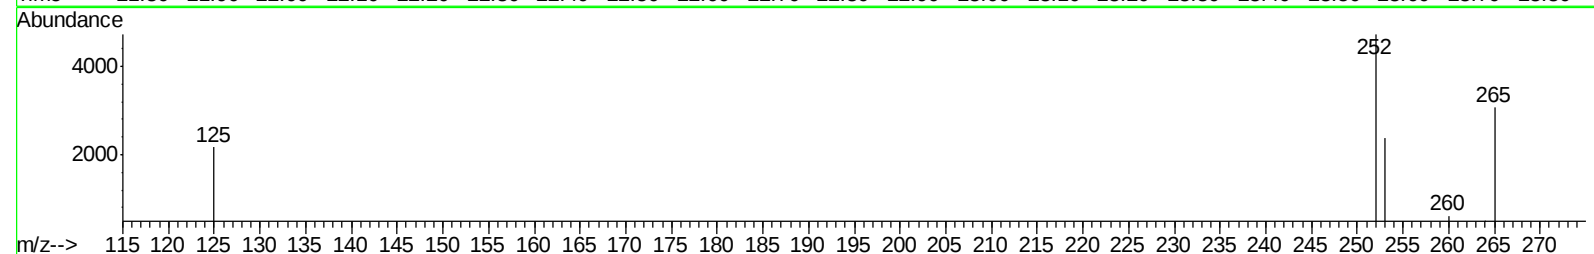


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012284.D
Acq On : 17 Oct 2020 01:30
Operator : CG/JU
Sample : L4201-08DL 5X
Misc :
ALS Vial : 96 Sample Multiplier: 1

Quant Time: Oct 17 03:21:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 23:42:05 2020
Response via : Initial Calibration

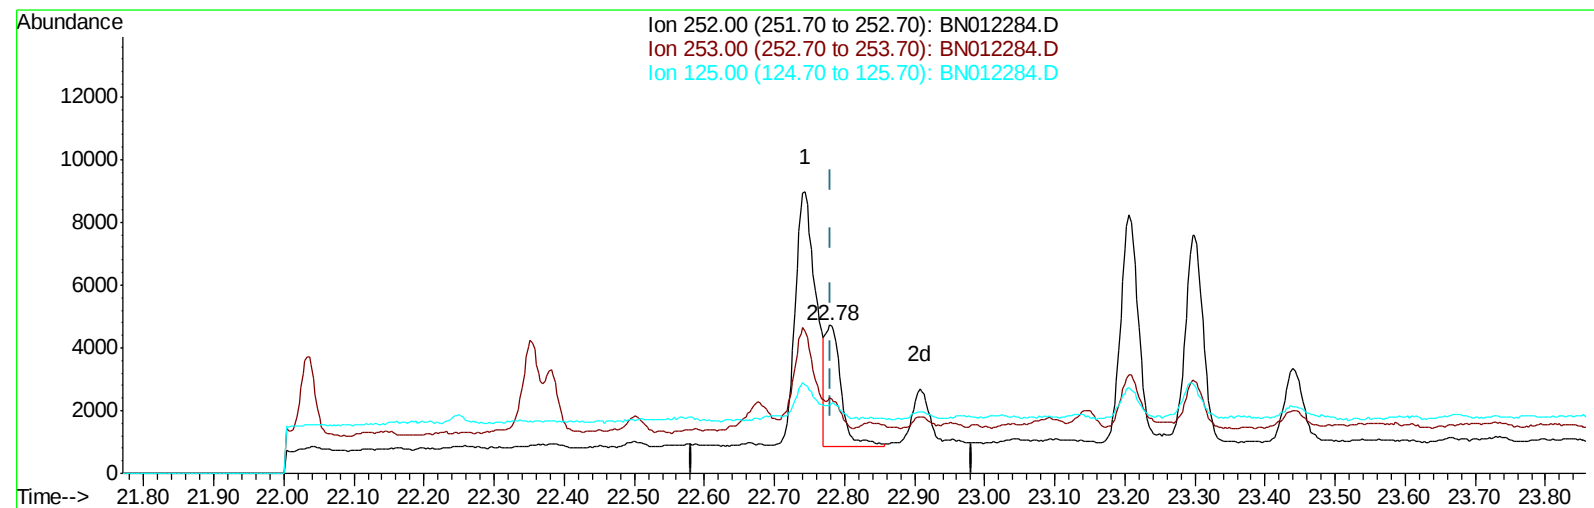

TIC: BN012284.D

(22) Benzo(k)fluoranthene

22.779min (-0.003) 0.19ng/ul m

response 6005

Ion	Exp%	Act%
252.00	100	100
253.00	30.50	50.62#
125.00	16.10	45.82#
0.00	0.00	0.00