

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012212.D
 Acq On : 15 Oct 2020 01:44
 Operator : CG/JU
 Sample : L4166-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB9

Quant Time: Oct 15 02:22:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 15 00:46:15 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1261	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	5077	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	3014	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.01
16) Chrysene-d12	21.21	240	5035	0.40	ng/ul	0.00
20) Perylene-d12	23.39	264	5943	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.00	152	1869	0.25	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	3967	0.00	ng/ul	0.00
Target Compounds				Ovalue		
7) Acenaphthylene	13.98	152	321	0.025	ng/ul#	62
17) Pyrene	19.44	202	866	0.038	ng/ul#	70
18) Benzo(a)anthracene	21.20	228	732	0.039	ng/ul#	78
19) Chrysene	21.24	228	1472	0.065	ng/ul	95
21) Benzo(b)fluoranthene	22.74	252	3089	0.129	ng/ul#	52
22) Benzo(k)fluoranthene	22.74	252	3089	0.116	ng/ul#	49
23) Benzo(a)pyrene	23.30	252	1458	0.062	ng/ul#	44
24) Indeno(1,2,3-cd)pyrene	25.57	276	985	0.033	ng/ul#	100
26) Benzo(g,h,i)perylene	26.24	276	991	0.036	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012212.D
Acq On : 15 Oct 2020 01:44
Operator : CG/JU
Sample : L4166-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB9

Quant Time: Oct 15 02:22:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 15 00:46:15 2020
Response via : Initial Calibration

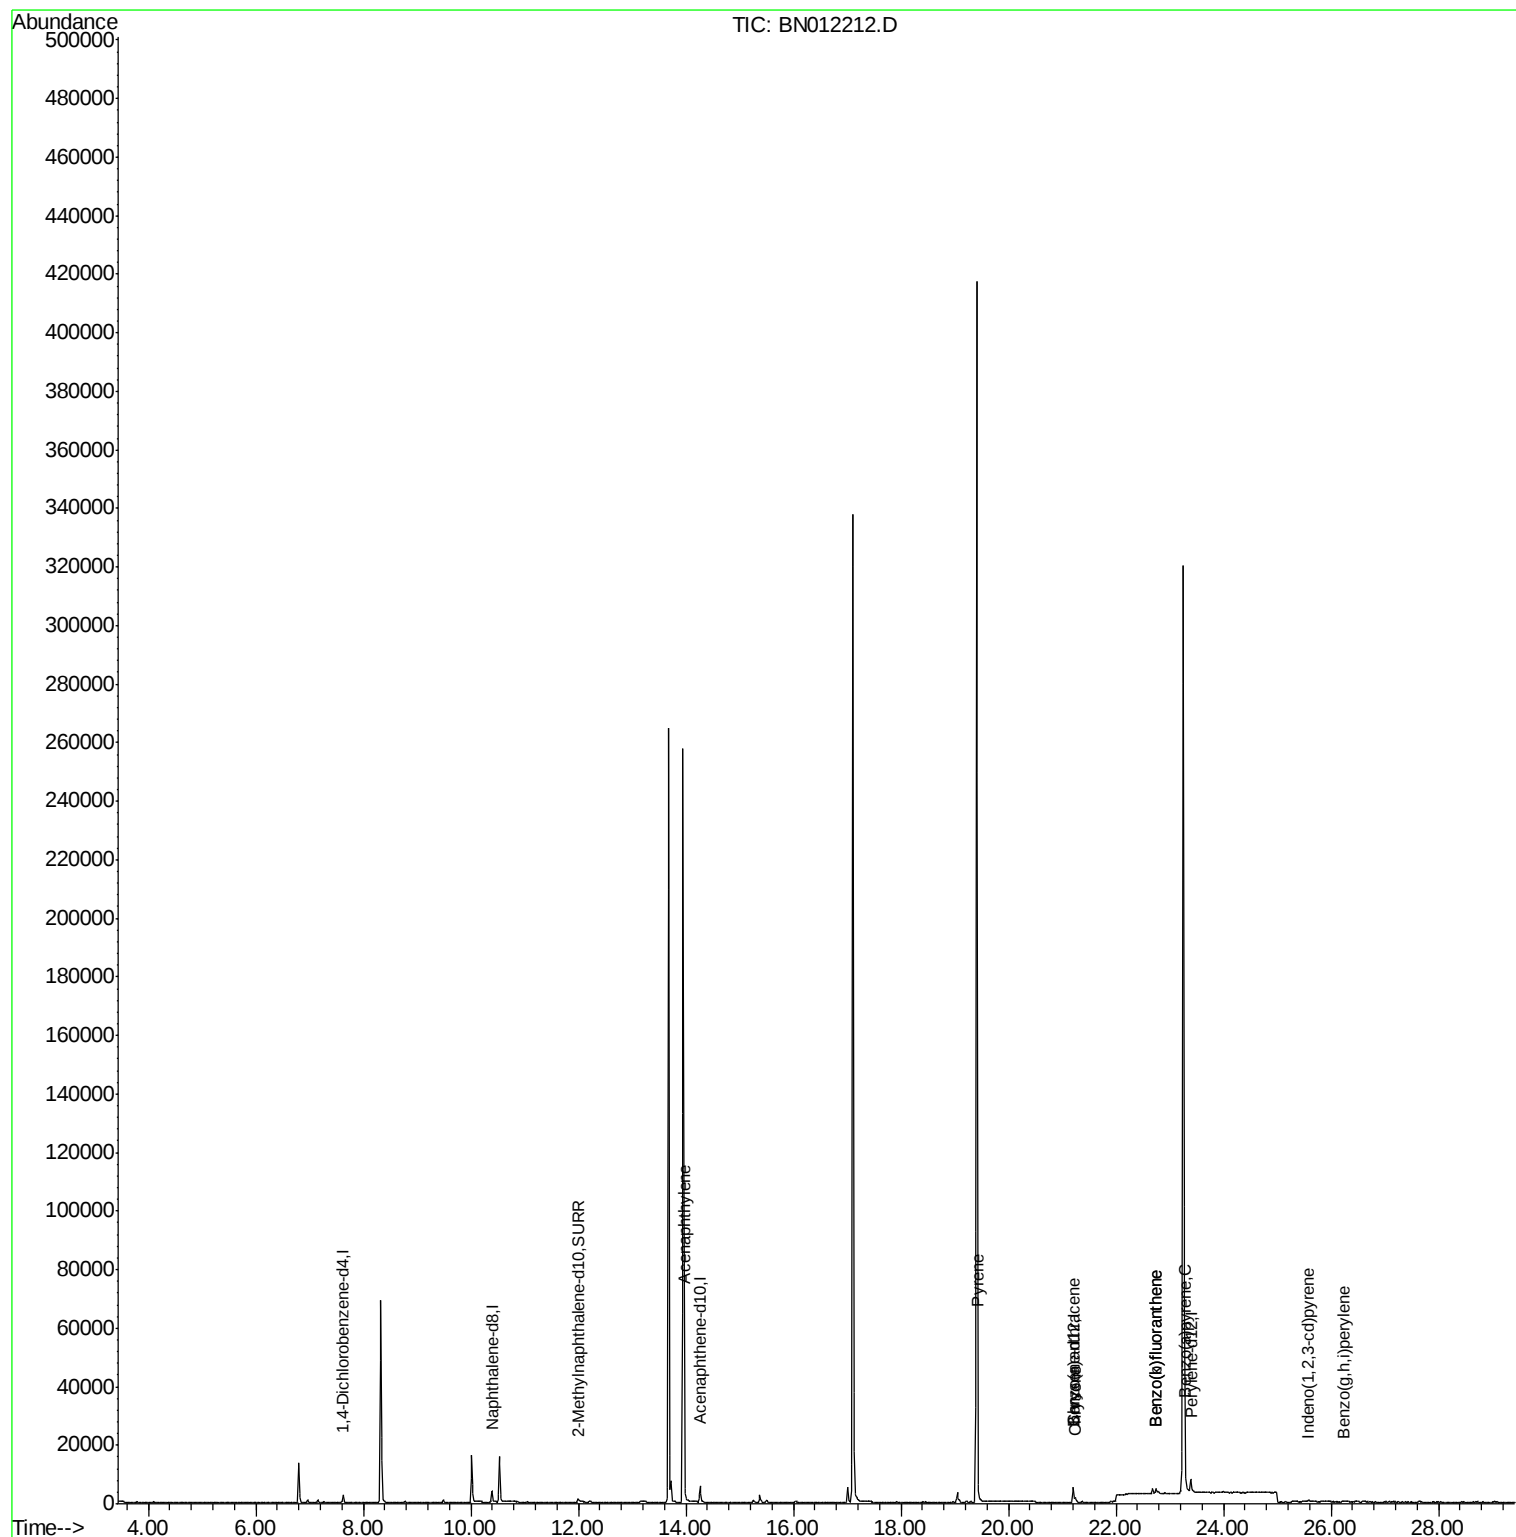

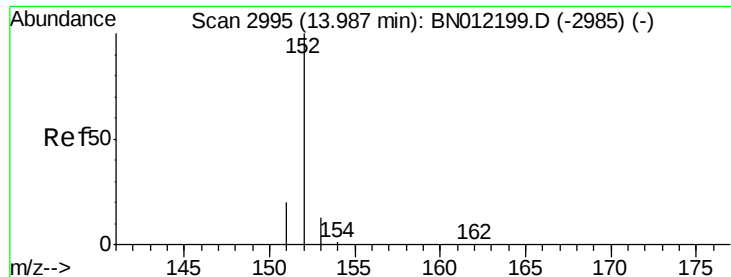

#7

Acenaphthylene

Concen: 0.025 ng/ul

RT: 13.98 min Scan# 2993

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44

Instrument :

BNA_N

ClientSampleId :

C0AB9


Tot Ion:152 Resp: 321

Ion Ratio Lower Upper

152 100

151 36.5 16.7 25.1#

153 33.0 11.8 17.8#

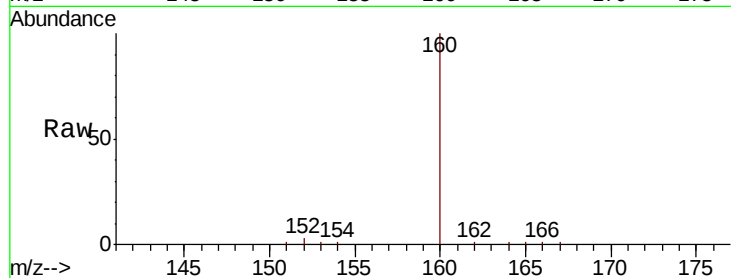



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

13.98

Time-->

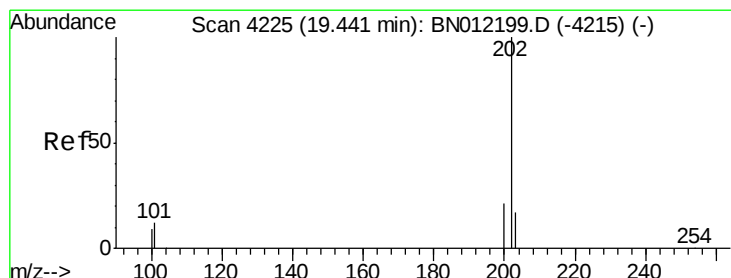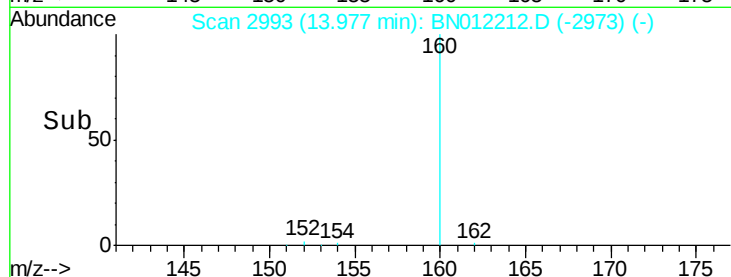

#17

Pyrene

Concen: 0.038 ng/ul

RT: 19.44 min Scan# 4224

Delta R.T. -0.00 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44


Tgt Ion:202 Resp: 866

Ion Ratio Lower Upper

202 100

101 21.1 9.9 14.9#

100 24.9 8.0 12.0#

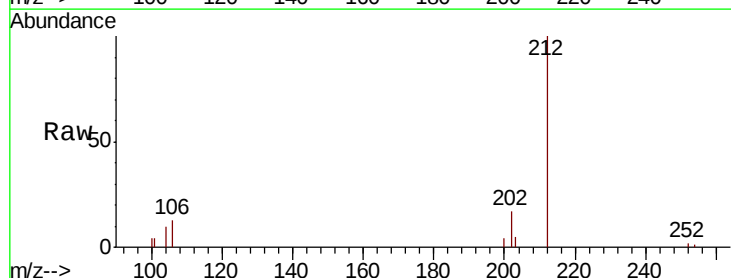


Abundance Ion 202.00 (201.70 to 202.70): E


Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

19.44

Time-->

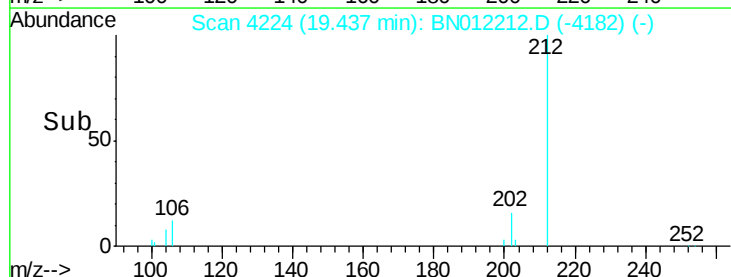

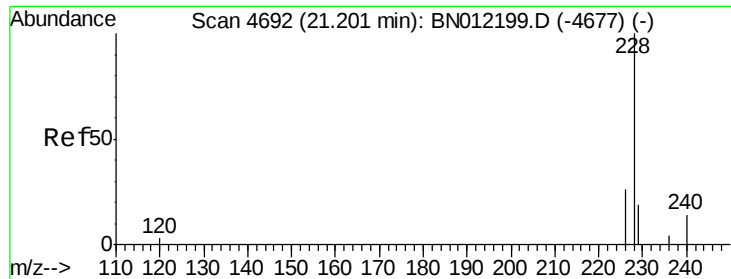

#18

Benzo(a)anthracene

Concen: 0.039 ng/ul

RT: 21.20 min Scan# 4690

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44

Instrument :

BNA_N

ClientSampled :

C0AB9


Tot Ion:228 Resp: 732

Ion Ratio Lower Upper

228 100

229 31.5 15.8 23.8#




226 38.0 22.6 33.8#

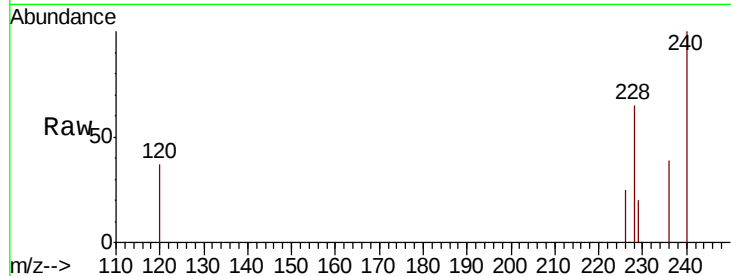

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

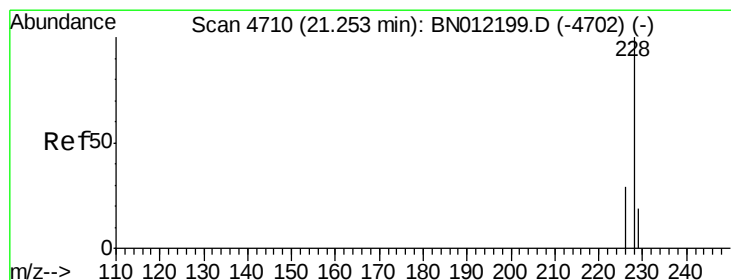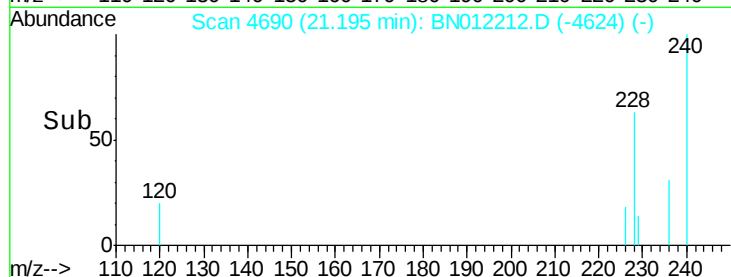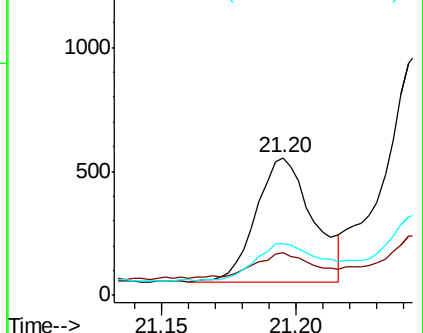

#19

Chrysene

Concen: 0.065 ng/ul

RT: 21.24 min Scan# 4707

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44


Tgt Ion:228 Resp: 1472

Ion Ratio Lower Upper

228 100

226 33.1 24.6 37.0



229 24.2 17.0 25.6

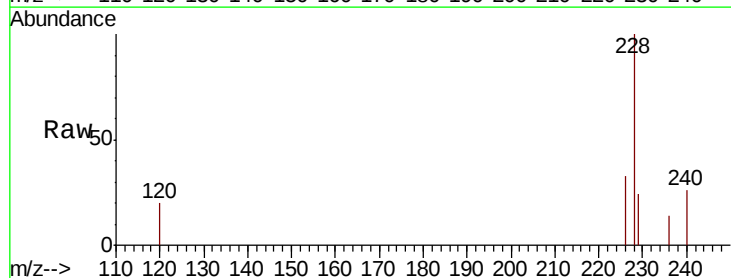


Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

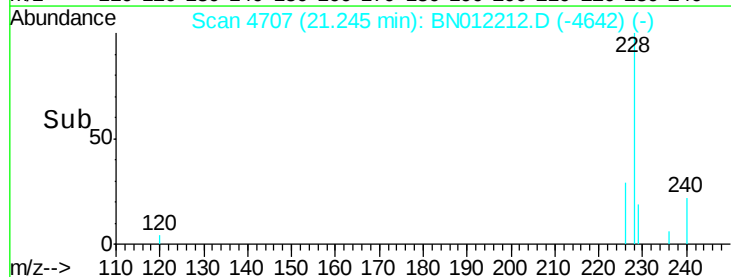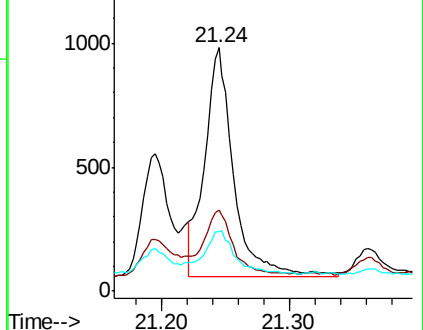

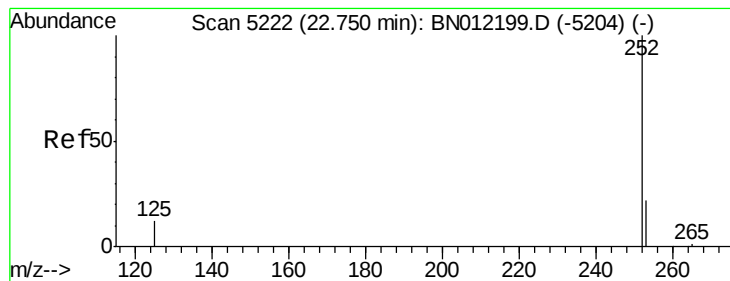

#21

Benzo(b)fluoranthene

Concen: 0.129 ng/ul

RT: 22.74 min Scan# 5219

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44

Instrument :

BNA_N

ClientSampleId :

C0AB9


Tot Ion:252 Resp: 3089

Ion Ratio Lower Upper

252 100

253 52.3 0.0 61.6




125 46.3 0.0 36.8#

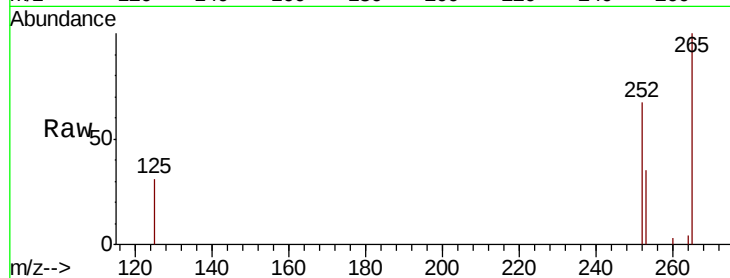

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

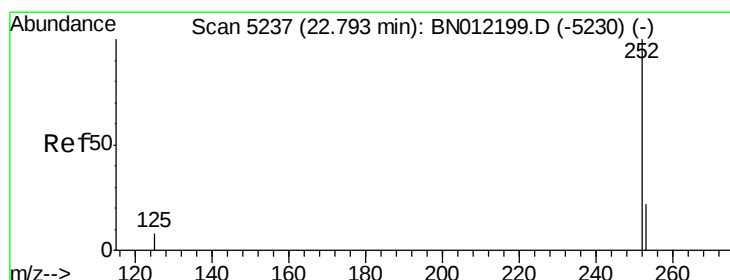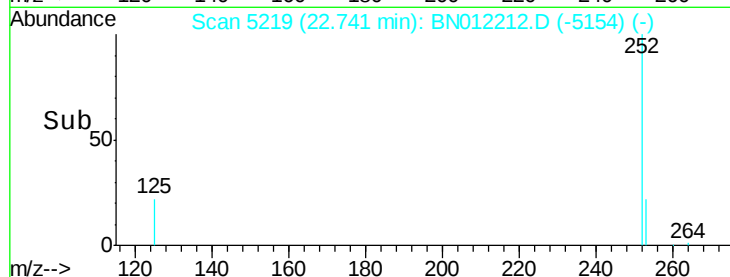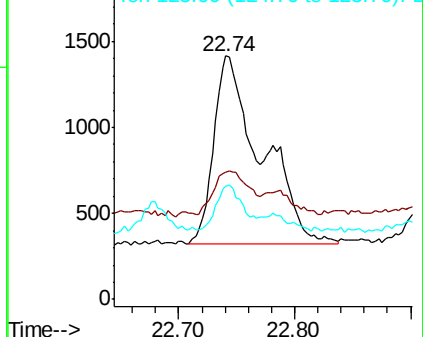

#22

Benzo(k)fluoranthene

Concen: 0.116 ng/ul

RT: 22.74 min Scan# 5219

Delta R.T. -0.05 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44


Tgt Ion:252 Resp: 3089

Ion Ratio Lower Upper

252 100

253 52.3 24.4 36.6#



125 46.3 12.9 19.3#

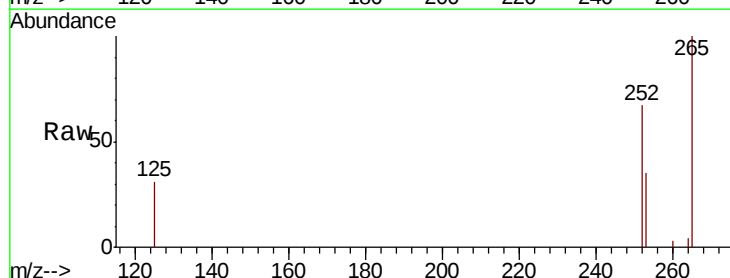


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

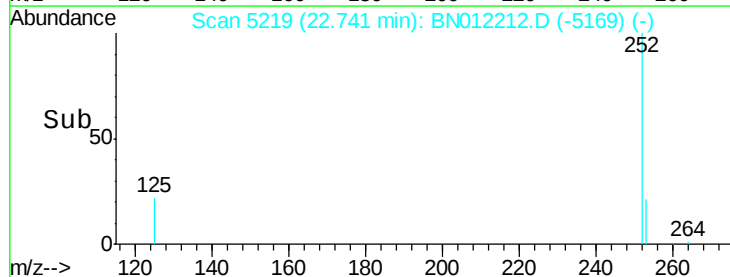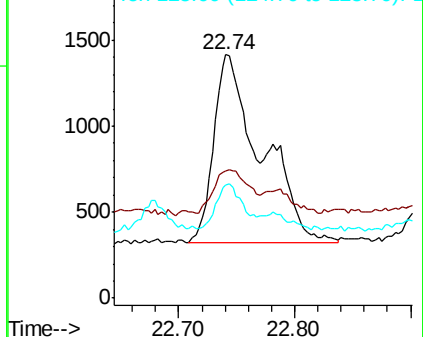

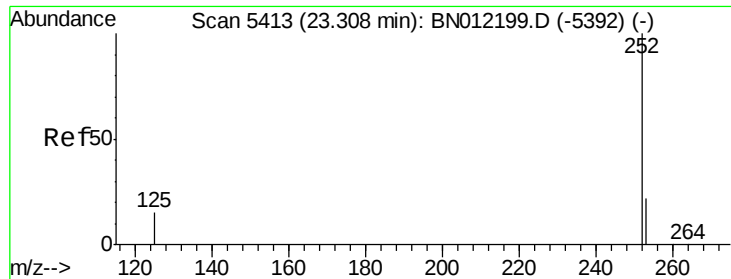

#23

Benzo(a)pyrene

Concen: 0.062 ng/ul

RT: 23.30 min Scan# 5409

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44

Instrument :

BNA_N

ClientSampleId :

C0AB9


Tot Ion:252 Resp: 1458

Ion Ratio Lower Upper

252 100

253 59.9 27.0 40.4#




125 57.8 18.8 28.2#

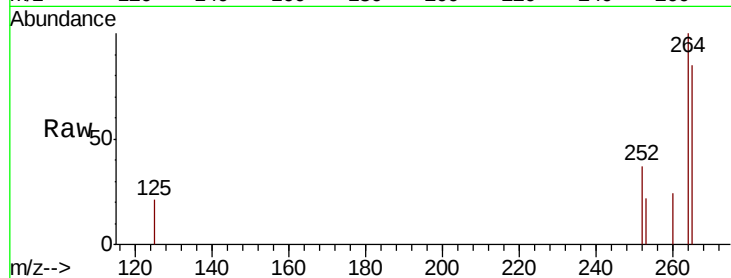

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

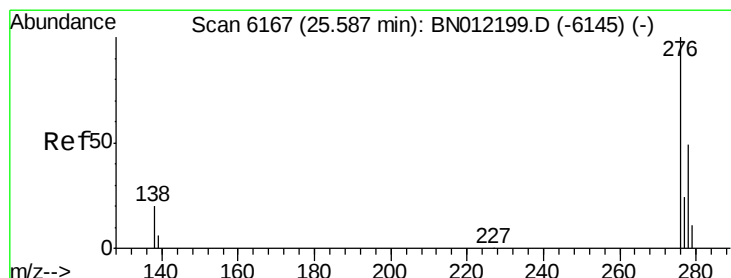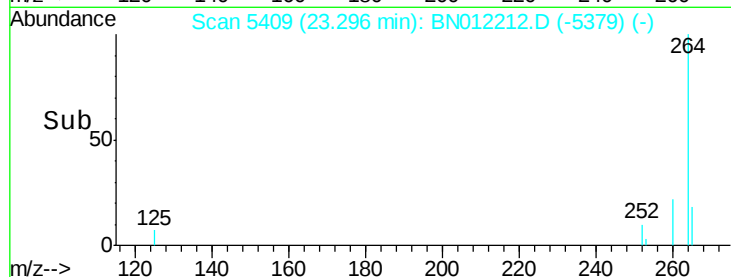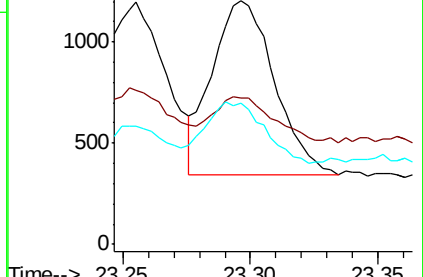

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.033 ng/ul

RT: 25.57 min Scan# 6163

Delta R.T. -0.01 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44


Tgt Ion:276 Resp: 985

Ion Ratio Lower Upper

276 100

138 27.7 0.0 0.0#



227 0.7 0.0 0.0#

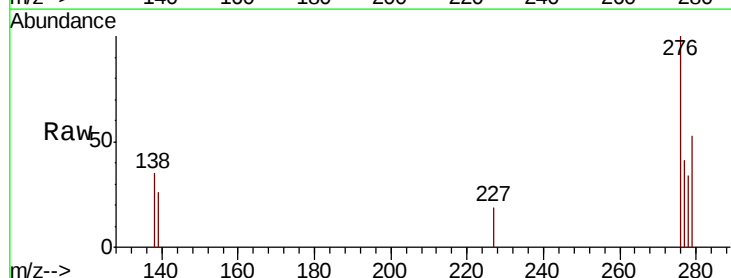


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

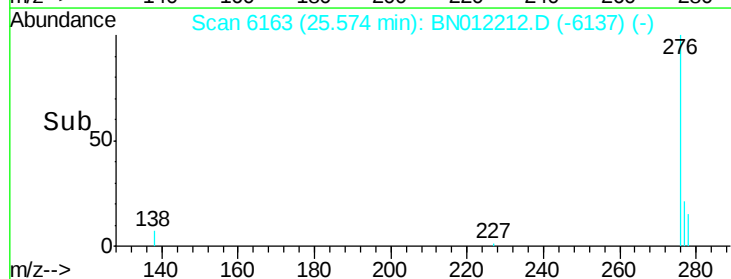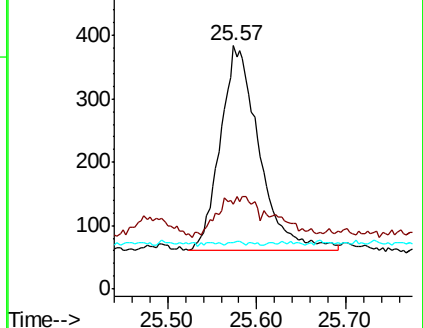

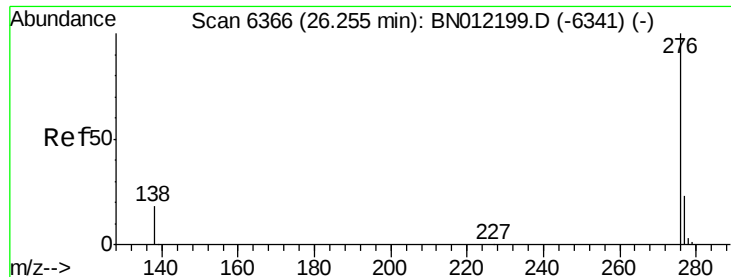

#26

Benzo(a,h,i)perylene

Concen: 0.036 ng/ul

RT: 26.24 min Scan# 6361

Delta R.T. -0.02 min

Lab File: BN012212.D

Acq: 15 Oct 2020 01:44

Instrument :

BNA_N

ClientSampleId :

C0AB9


Tot Ion: 276 Resp: 991

Ion Ratio Lower Upper

276 100

138 37.5 17.1 25.7#

277 41.9 21.1 31.7#

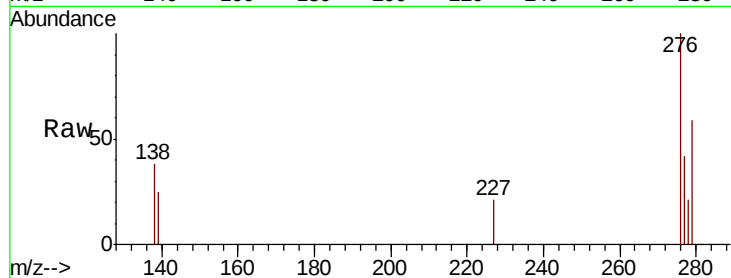

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

