

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012239.D
 Acq On : 15 Oct 2020 19:48
 Operator : CG/JU
 Sample : L4235-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN5

Quant Time: Oct 16 01:27:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:19:50 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1786	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	7527	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	4457	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.01
16) Chrysene-d12	21.21	240	7929	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	8434	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	2992	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	6687	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.41	202	1416	0.040	ng/ul#	1
23) Benzo(a)pyrene	23.26	252	2424	0.073	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012239.D
Acq On : 15 Oct 2020 19:48
Operator : CG/JU
Sample : L4235-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN5

Quant Time: Oct 16 01:27:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration




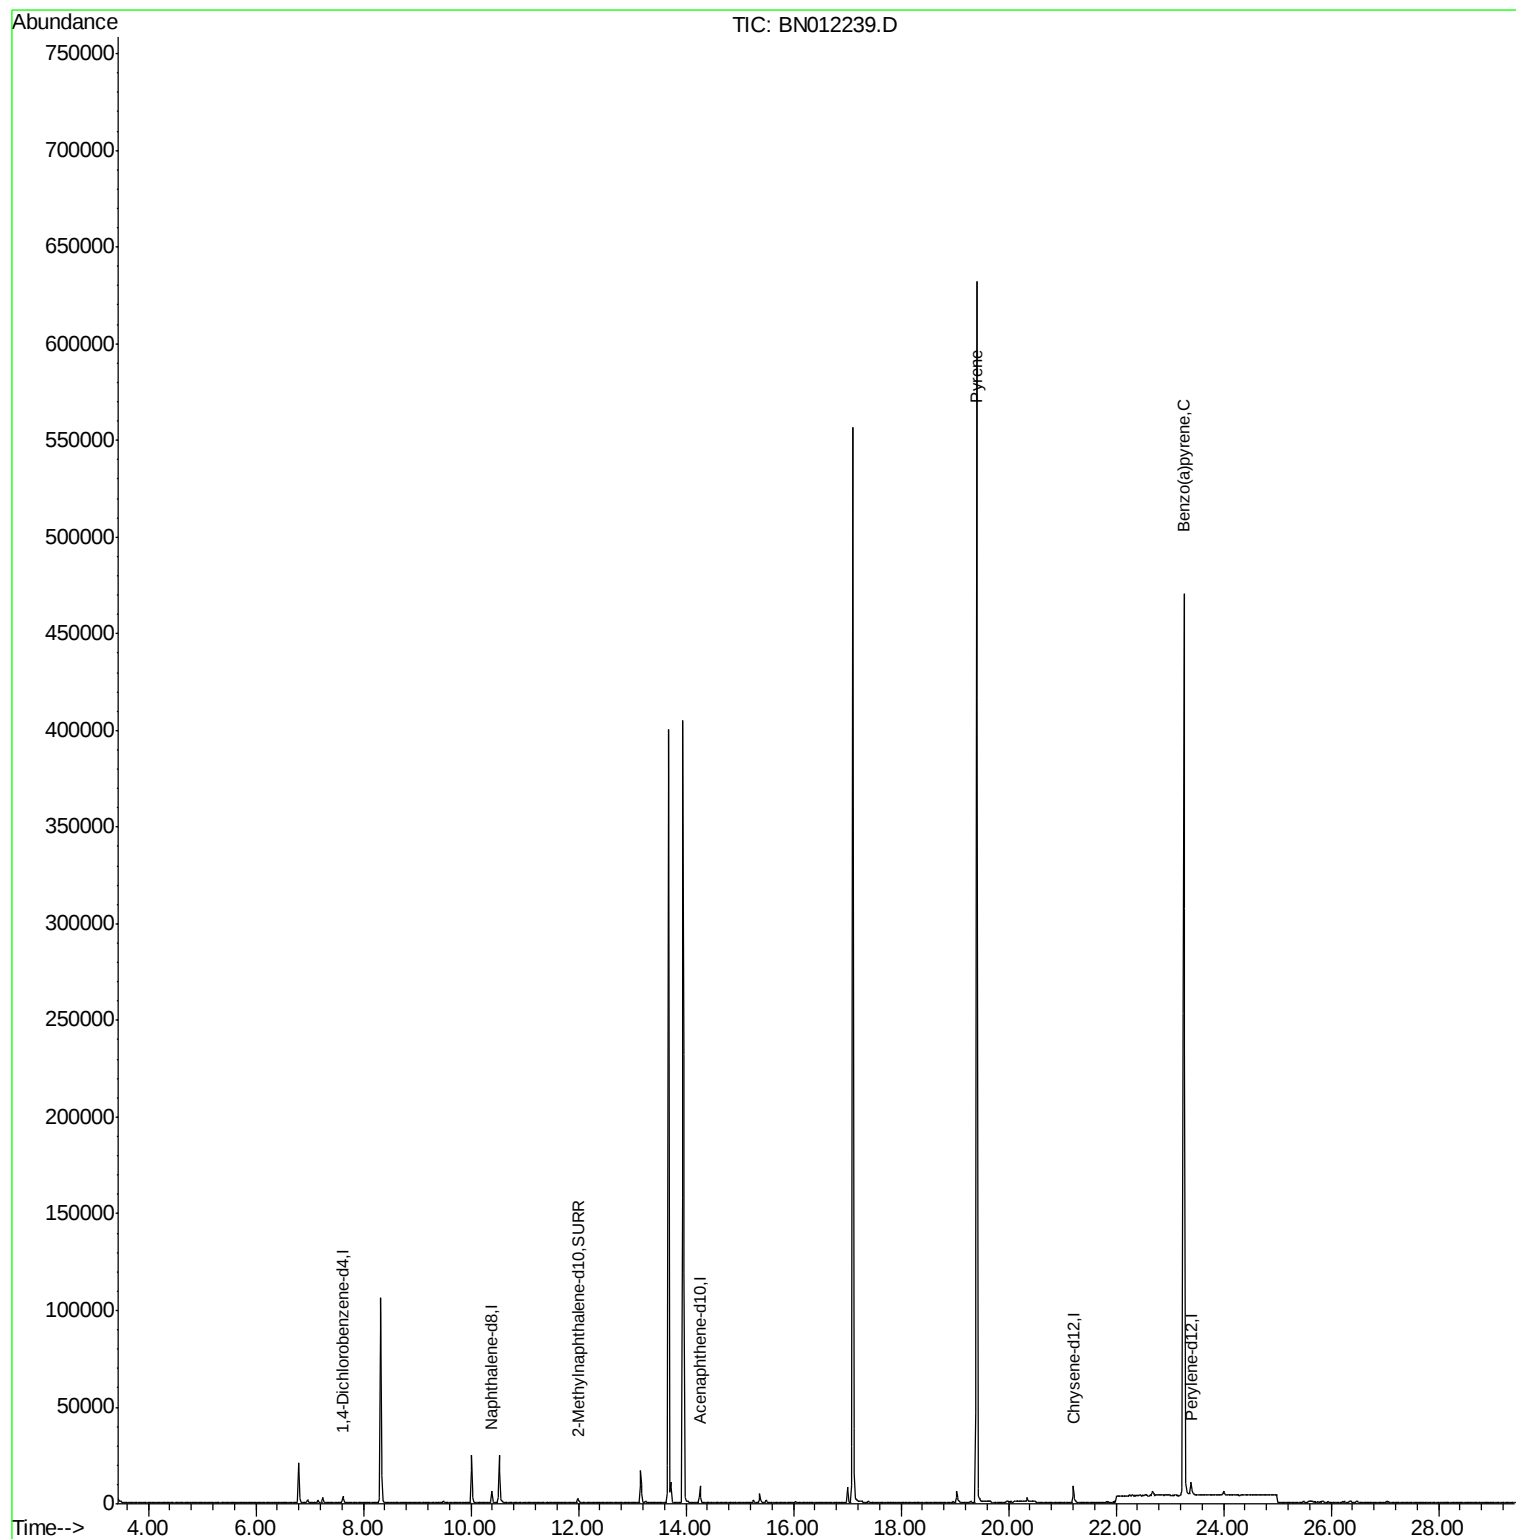


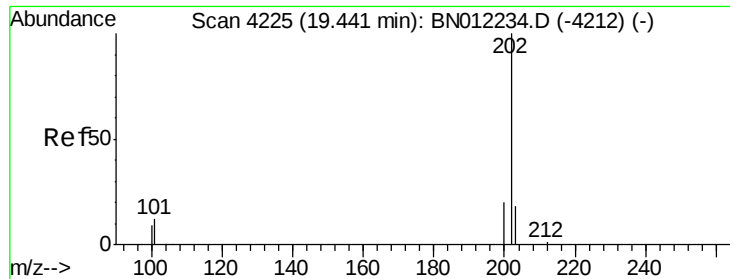

#17
Pvrene
Concen: 0.040 ng/ul
RT: 19.41 min Scan# 4218
Delta R.T. -0.03 min
Lab File: BN012239.D
Acq: 15 Oct 2020 19:48

Instrument :
BNA_N
ClientSampleId :
C0AN5

Tot Ion:202 Resp: 1416
Ion Ratio Lower Upper
202 100
101 179.6 9.9 14.9#
100 1208.7 8.0 12.0#

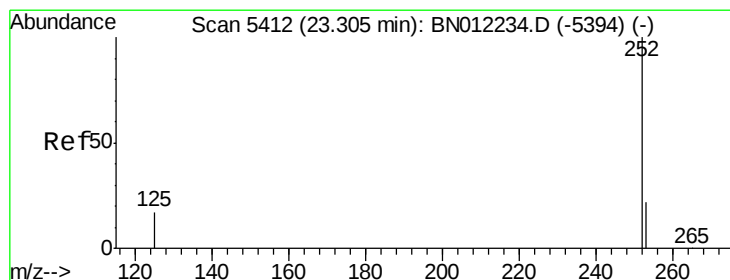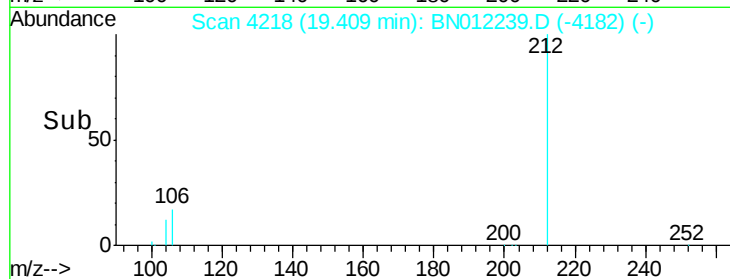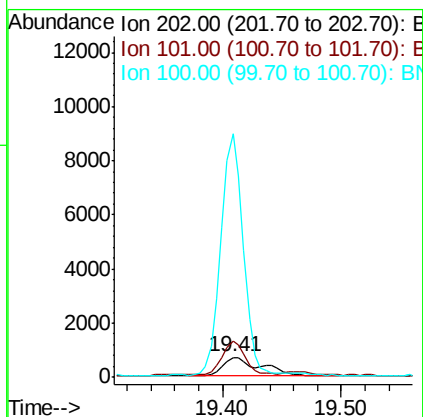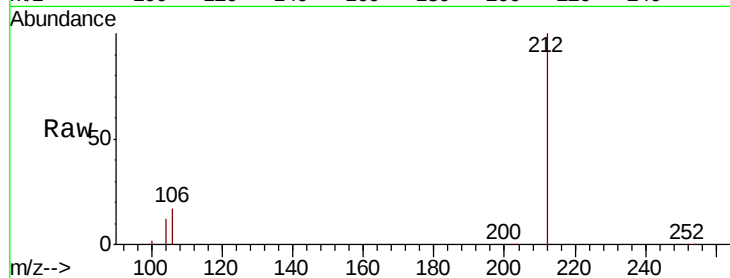

#23
Benzo(a)pyrene
Concen: 0.073 ng/ul
RT: 23.26 min Scan# 5397
Delta R.T. -0.04 min
Lab File: BN012239.D
Acq: 15 Oct 2020 19:48

Tgt Ion:252 Resp: 2424
Ion Ratio Lower Upper
252 100
253 60.9 27.0 40.4#
125 53.3 18.8 28.2#

