


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012239.D
Acq On : 15 Oct 2020 19:48
Operator : CG/JU
Sample : L4235-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN5

Manual Integrations
APPROVED

mohammad
10/19/2020 1:19:59 PM

Quant Time: Oct 16 01:39:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

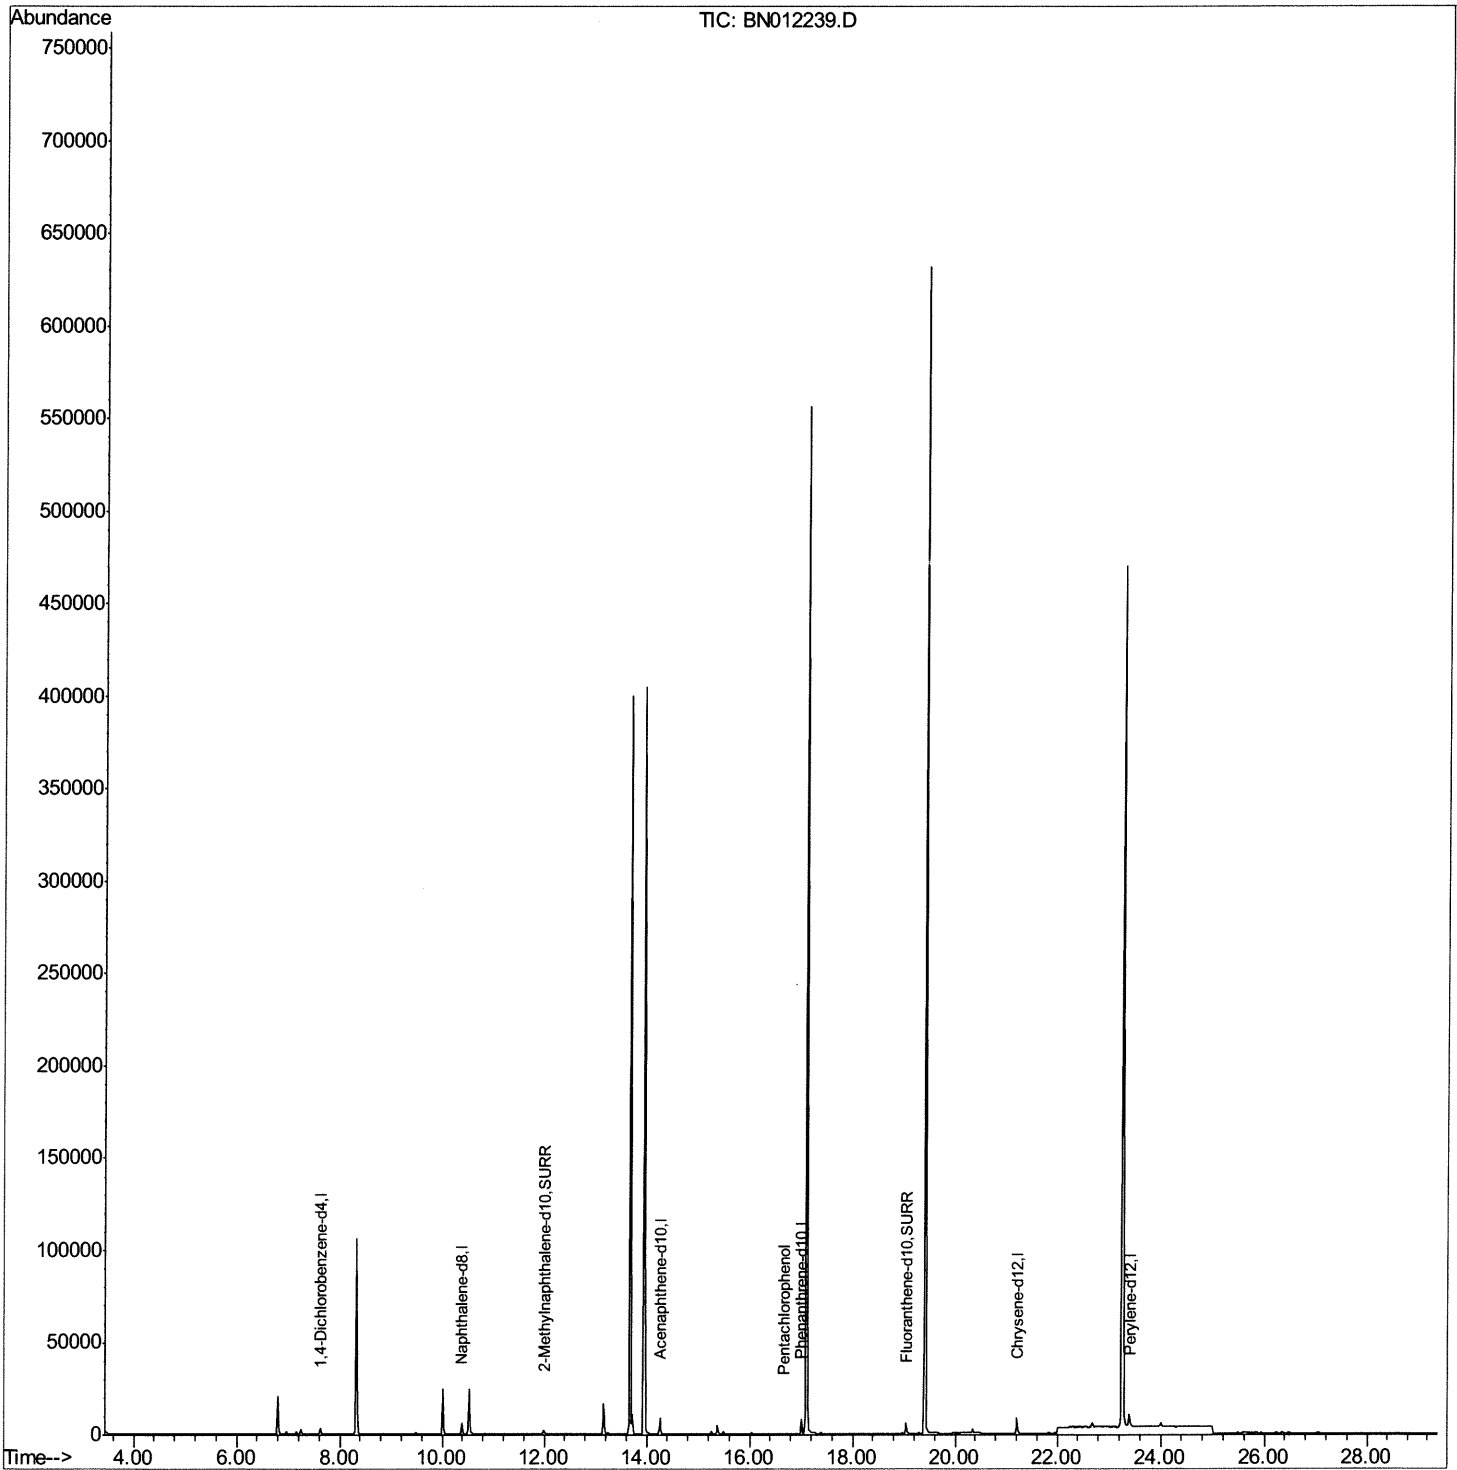

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012239.D
Acq On : 15 Oct 2020 19:48
Operator : CG/JU
Sample : L4235-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN5

Manual Integrations
APPROVED

mohammad
10/19/2020 1:19:59 PM

Quant Time: Oct 16 01:27:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

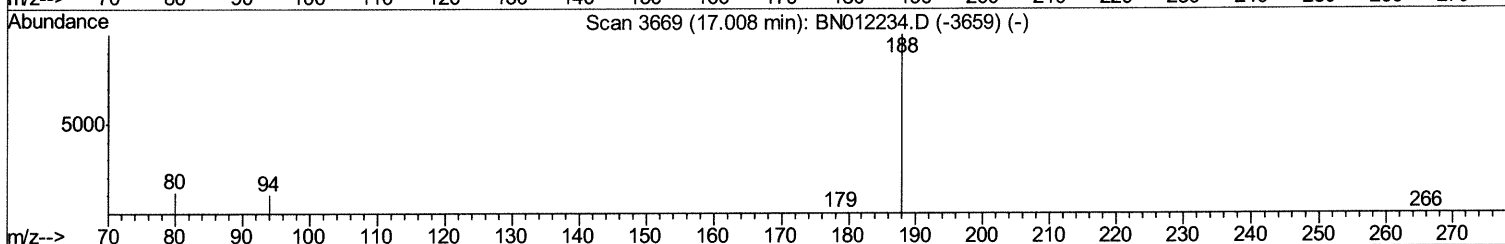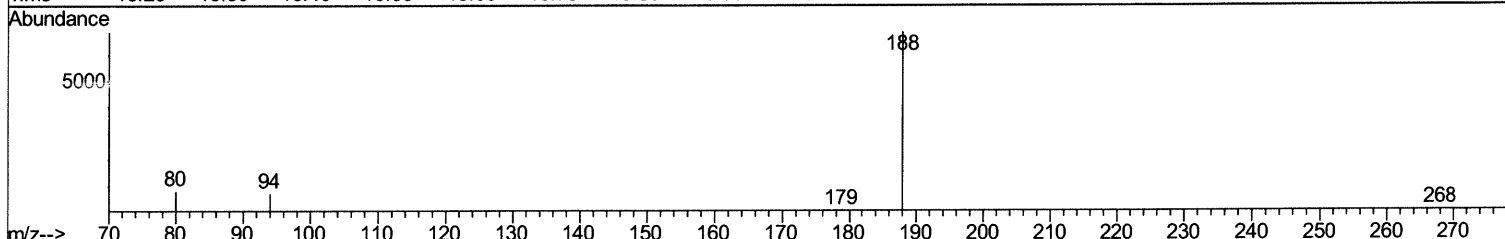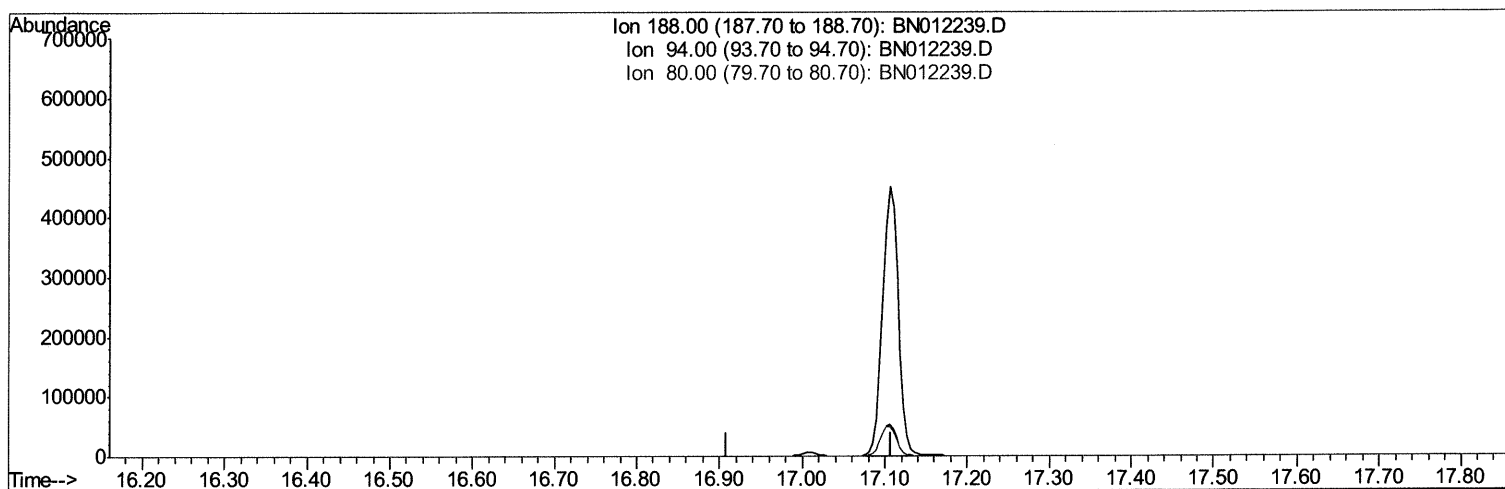

TIC: BN012239.D

(10) Phenanthrene-d10 (I)

17.008min (-17.008) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	11.20	0.00#
80.00	12.20	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
Data File : BN012239.D
Acq On : 15 Oct 2020 19:48
Operator : CG/JU
Sample : L4235-04
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AN5

Manual Integrations
APPROVED

mohammad
10/19/2020 1:19:59 PM

Quant Time: Oct 16 01:27:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 16 01:19:50 2020
Response via : Initial Calibration

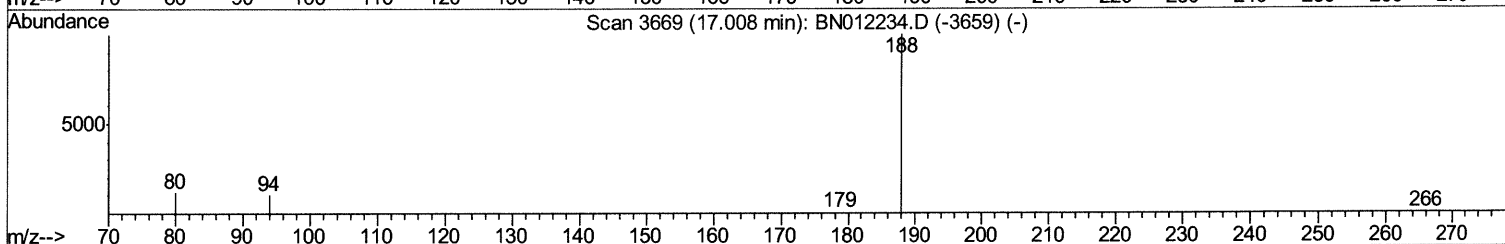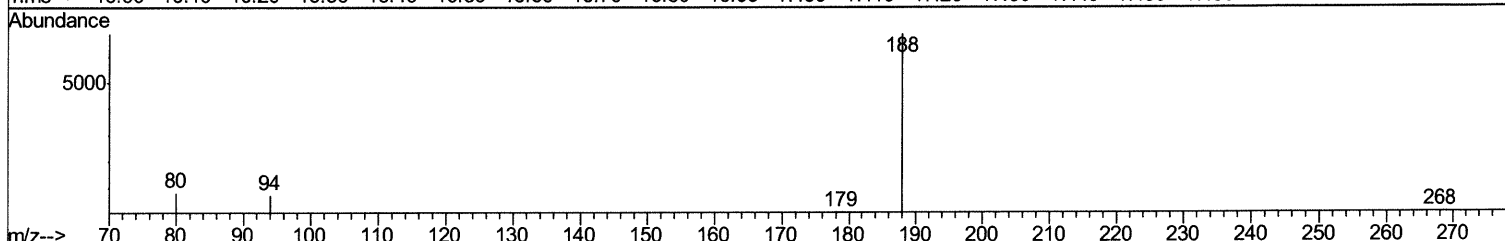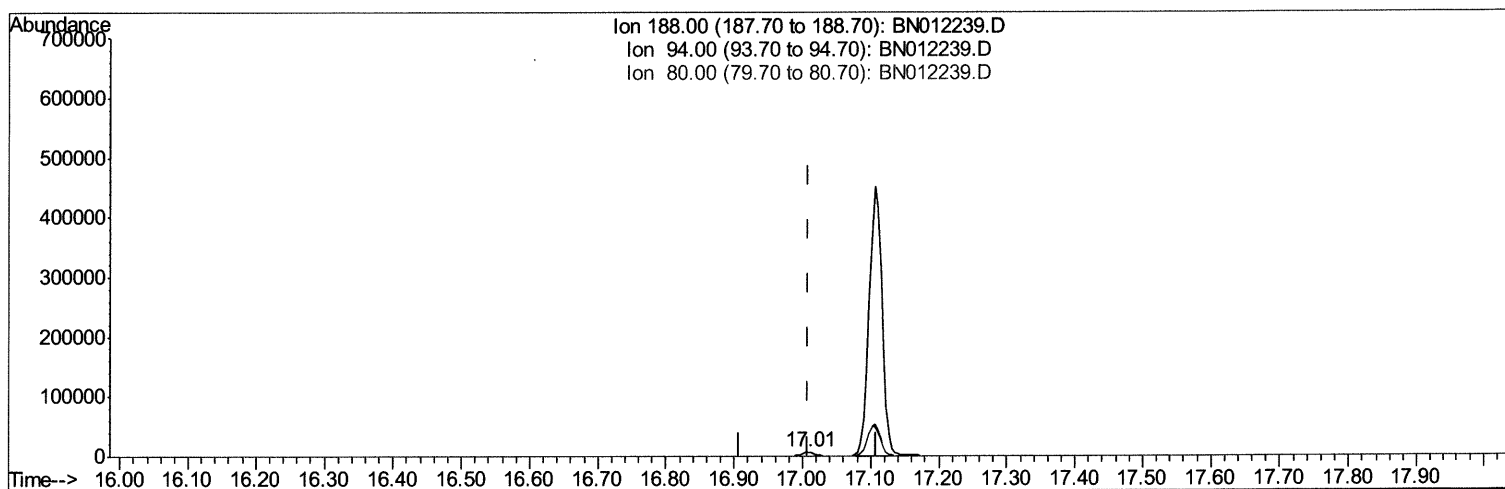

TIC: BN012239.D

(10) Phenanthrene-d10 (I)

17.009min (+0.000) 0.40ng/ul m 10/20/20 JU

response 9394

Ion	Exp%	Act%
188.00	100	100
94.00	11.20	10.57
80.00	12.20	11.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN101420\
 Data File : BN012239.D
 Acq On : 15 Oct 2020 19:48
 Operator : CG/JU
 Sample : L4235-04
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AN5

Manual Integrations
 APPROVED

mohammad
 10/19/2020 1:19:59 PM

Quant Time: Oct 16 01:39:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN101420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 16 01:19:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	1786	0.40	ng/ul	0.00
2) Naphthalene-d8	10.39	136	7527	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.26	164	4457	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	9394m >	0.40	ng/ul >	0.00 10/20/20 SQ
16) Chrysene-d12	21.21	240	7929	0.40	ng/ul	0.00
20) Perylene-d12	23.40	264	8434	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.99	152	2992	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.04	212	6687	0.26	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.66	266	63	0.023	ng/ul	Ovalue 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed